

INTOXILYZER® 8000 INITIAL INSPECTION

Serial Number: 80-005948

1. Power On and Warm-up:

- a. Power On
- b. 5 min. Countdown from Initial Warm-up
- c. 1 min. Countdown to Begin a Test
- d. Forms Load Complete

2. Setup and Checks:

a. Level 1:

- 1) Passwords: Field Inspector (Level 2) Lab Personnel (Level 3)
- 2) Gas Cylinder: Gas Cylinder Setup (Level 1,S)
- 3) Printer: Printer Setup (Level 3,S,P)
 - Internal Printer Paper Feed
 - Internal Printer Test (Level 1,P)
 - External Printer Test (Level 1,P)
- 4) Barcode Reader (Level 1,B): Operator ID
 ND License

b. Level 2:

- 1) Continuous Purge (Level 2,A)
- 2) Diagnostic (Level 2,D)
- 3) Prelim Data Entry (Level 2,E)
- 4) Ser Num/Version Info (Level 2,V): Ser Num 80-005948
Version 8164.13

c. Level 3:

- 1) DVM Monitor (Level 3,D,D): 3: 12646 s: 0 C: 47.00
9: 13278 s: 1 B: 45 0
(RFI indicator with keyed radio) 1
- 2) Function (F) Keys: F5 – Tone
 F6 – Green LED
 F7 – Red LED
 F9 – Fan
 F10 – Pump
 F11 – Solenoid *A CEC*
- 3) Atmospheric Monitor (Level 3,D,T): Atmo Sensor, P: 957 CF: 1.05
- 4) Flow Monitor (Level 3,D,F): Flow Sensor, R: 229 F: 0.000 L/s

5) Temperature Monitor (Level 3,D,T): C: 47.0 A: 47.5 I: 0.0
B: 45.0 V: 0.0

6) Tank Monitor (Level 3,D,G): P (gauge): 260 P (display): 261
7) General Setup (Level 3,S,G)
8) Configure Start Test (Level 3,S,T)
9) Network (Level 3,S,N)

3. Tests:

a. Configure Standard for Wet Bath Simulator (Level 1,S):

1) Zero Alcohol Test (Level 1,C):

Sim Ser #: DR5188 Lot #: NA Exp Date: NA
Known Value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC

2) Low AC Test (Level 1,C):

Sim Ser #: DR3455 Lot #: 12210 Exp Date: 11-2-14
Known Value: 0.020 AC
Results: 0.019 AC 0.020 AC 0.020 AC

3) Linearity Test (Level 1,C):

Sim Ser #: DR3847 Lot #: 13020 Exp Date: 1-15-15
Known Value: 0.300 AC
Results: 0.299 AC 0.301 AC 0.302 AC

b. Configure Dry Gas Standard (Level 1,S):

1) Interferent Detected Tests (Level 1,B):

1. 0.10 AC + 0.05% Acetone

Sim Ser #: DR3377 Lot #: ICS#1 Exp Date: 4-9-14
Known Value: 0.10AC + 0.05% ACETONE
 Display reads "Interferent Detect"

2. Acetone

Sim Ser #: GB919 Lot #: ACE 1 Exp Date: 8-27-15
4-9-CEE
Known Value: 0.05% ACETONE
 Display reads "Interferent Detect"

3. Methanol

Sim Ser #: G10573 Lot #: MET 1 Exp Date: 8-27-15
Known Value: 0.10% METHANOL
 Display reads "Interferent Detect"

4. Isopropanol
Sim Ser #: G9998 Lot #: IPA1 Exp Date: 8-27-15
Known Value: 0.10% ISOPROPANOL
 Display reads "Interferent Detect"
- 2) Ambient Fail (Level 1,B): Display and test record are correct
3) Invalid Sample (Level 1,B): Display and test record are correct
4) Subject Test Timeout (Level 1,B): Display and test record are correct.
5) Sequence Aborted (Level 1,B): Display and test record are correct
6) Control Outside Tolerance (CMS mode): Display and test record are correct
7) RFI Detected Test (CMS mode): Display and test record are correct
8) Tank Pressure Below Min (CMS mode): Display reads correct
9) Subject Refused (CMS mode): Display and test record are correct
10) Difference Too Great (CMS mode): Display and test record are correct
11) Stability Test (Level 3,T,S):
Average 0.0810 Std Dev 0.0006 Rel Std Dev 0.75%

Maintenance/Repairs/Notes: _____

THIS UNIT IS ACCEPTABLE TO BE USED IN THE FIELD

Charles E. Edr
Field Inspector's Signature

9/9/13
Date

Deb Kashner
Reviewed by

11 Sept 2013 ✓
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 10:41

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQRSTUWX

32 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQRSTUWXYZ1234567890ABCDEF

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On MemFull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 23411080A1
Standard Cyl #? 55
Standard Expiration? 10/01/2013
Oper No? 666666

Flow Cal. Date: 06/20/2013
Slope 701
Intercept -716431

IR Calibration Date: 06/20/2013
Sum Sum

0th Coef(*100):	-26846	-20297
1st Coef(*100):	287817	140427
2nd Coef(*100):	316	919
H2O adj(mg/l)*10K):	604	447

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: INTERNAL
PRINT
TEST

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 10:44

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 23411080A1
Standard Cyl #? 55
Standard Expiration? 10/01/2013
Oper No? 666666

Flow Cal. Date: 06/20/2013
Slope 701
Intercept -716431

IR Calibration Date: 06/20/2013

	3um	9um
0th Coef(*100):	-26846	-20297
1st Coef(*100):	287817	140427
2nd Coef(*100):	316	919
H2O adj(mg/l*10k):	604	447

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

EXTERNAL PRINT
TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 10:50

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *DIAGNOSTIC CHECK*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 11:27

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:28
02 Std. Sol.	0.000	11:29
03 Room Air	0.000	11:29
04 Std. Sol.	0.000	11:30
05 Room Air	0.000	11:30
06 Std. Sol.	0.000	11:31
07 Room Air	0.000	11:31

08 Sim Temp = 34.0°C

Simul Ser No = DR5188
Std Sol No = MILLIQH2O
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: ZERO ALCOHOL TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 13:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:15
02 Std. Sol.	0.019	13:16
03 Room Air	0.000	13:16
04 Std. Sol.	0.020	13:17
05 Room Air	0.000	13:18
06 Std. Sol.	0.020	13:18
07 Room Air	0.000	13:19

08 Sim Temp = 34.0°C

Simul Ser No = DR3455

Std Sol No = 12210

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: 0.020 AC Sim. Sol
Low AC TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 13:22

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:23
02 Std. Sol.	0.299	13:23
03 Room Air	0.000	13:24
04 Std. Sol.	0.301	13:25
05 Room Air	0.000	13:25
06 Std. Sol.	0.302	13:26
07 Room Air	0.000	13:27

08 Sim Temp = 34.0°C

Simul Ser No = DR3847

Std Sol No = 13020

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *LINEARITY TEST*
0.300 AC SIM. SOL.


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 13:57

Test	AC	Time
01 Room Air	0.000	13:58
02 *Subject Test	INT*	13:59
03 Room Air	0.000	13:59

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.10AC+0.05ACE
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INTERFERENT CHECK*
0.10AC + 0.05% ACETONE


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:08

Test	AC	Time
01 Room Air	0.000	14:09
02 *Subject Test	INT*	14:09
03 Room Air	0.000	14:10

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.05ACETONE
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INTERFERENT TEST*

0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:11

Test	AC	Time
01 Room Air	0.000	14:12
02 *Subject Test	INT*	14:13
03 Room Air	0.000	14:13

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.10METHANOL
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: 0.10% METHANOL
 INTERFERENT CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:15

Test	AC	Time
01 Room Air	0.000	14:16
02 *Subject Test	INT*	14:16
03 Room Air	0.000	14:17

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.10ISOPROPANOL
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INTERFERENT CHECK*
0.10% ISOPROPANOL

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:27

Test	AC	Time
01 Room Air	AMB*	14:29
02 Room Air	0.000	14:30

*Invalid Test
 Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *AMBIENT FAIL CHECK*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:40

Test	AC	Time
01 Room Air	0.000	14:41
02 Invalid Sample	X.XXX	14:41
03 Room Air	0.000	14:42

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

INVALID SAMPLE CHECK


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:43

Test	AC	Time
01 Room Air	0.000	14:44
02 *Subject Test	0.000*	14:47
03 Room Air	0.000	14:47
No RFI Detected		

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SUBJECT TIMEOUT
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *SUBJECT TEST TIMEOUT CHECK*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:48

Test	AC	Time
01 Room Air	0.000	14:49
02 *Subject Test	ABT*	14:49
03 Room Air	0.000	14:50

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SEQUENCE ABORT
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: SEQUENCE ABORTED CHECK

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 14:52

Test	AC	Time
01 Diagnostic	OK	14:53
02 Room Air	0.000	14:54
03 Subject Test 1	0.000	14:54
04 Room Air	0.000	14:56
05 Std. Gas	0.081*	14:57
06 Room Air	0.000	14:58

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CONTROL OUT TOL
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CONTROL OUT OF TOLERANCE
CHECK

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 15:03

Test	AC	Time
01 Diagnostic	OK	15:04
02 Room Air	RFI*	15:05
03 Room Air	0.000	15:05

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI DETECTED
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 15:11

Test	AC	Time
01 Diagnostic	OK	15:12
02 Room Air	0.000	15:12
03 *Subject Test	0.000*	15:15
04 Room Air	0.000	15:18
05 Std. Gas	0.081	15:19
06 Room Air	0.000	15:20
07 *Subject Test	REF**	15:20
08 Room Air	0.000	15:21

*Deficient Sample - Value Printed was
Highest Obtained
**Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SUBJECT REFUSED
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.

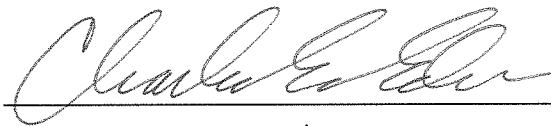

Operator Signature
CHARLES EDER

Remarks: *SUBJECT REFUSED TEST*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 15:25

Test	AC	Time
01 Diagnostic	OK	15:27
02 Room Air	0.000	15:27
03 Subject Test 1	0.000*	15:28
04 Room Air	0.000	15:30
05 Std. Gas	0.080	15:31
06 Room Air	0.000	15:33
07 Subject Test 2	0.102*	15:33
08 Room Air	0.000	15:34

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DIFFERENCE >
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 55
Expiration Date = 10/01/2013
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *DIFFERENCE TOO GREAT*
CHECK

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005948
Location = TOXL 8164.13.00 06/09
09/05/2013 15:39

Test	AC	Time
01 Room Air	0.000	15:40
02 Std. Gas	0.081	15:40
03 Room Air	0.000	15:41
04 Std. Gas	0.080	15:41
05 Room Air	0.000	15:41
06 Std. Gas	0.081	15:42
07 Room Air	0.000	15:42
08 Std. Gas	0.081	15:43
09 Room Air	0.000	15:43
10 Std. Gas	0.082	15:44
11 Room Air	0.000	15:44
12 Std. Gas	0.080	15:44
13 Room Air	0.000	15:45
14 Std. Gas	0.081	15:45
15 Room Air	0.000	15:46
16 Std. Gas	0.081	15:46
17 Room Air	0.000	15:47
18 Std. Gas	0.081	15:47
19 Room Air	0.000	15:48
20 Std. Gas	0.081	15:48
21 Room Air	0.000	15:49
22 Std. Gas	0.080	15:49
23 Room Air	0.000	15:49
24 Std. Gas	0.080	15:50
25 Room Air	0.000	15:50
26 Std. Gas	0.082	15:51
27 Room Air	0.000	15:51
28 Std. Gas	0.081	15:52
29 Room Air	0.000	15:52
30 Std. Gas	0.081	15:52
31 Room Air	0.000	15:53
32 Std. Gas	0.081	15:53
33 Room Air	0.000	15:54
34 Std. Gas	0.081	15:54
35 Room Air	0.000	15:55
36 Std. Gas	0.081	15:55
37 Room Air	0.000	15:56
38 Std. Gas	0.082	15:56
39 Room Air	0.000	15:57
40 Std. Gas	0.081	15:57
41 Room Air	0.000	15:57
42 Cal Check Stats:		
43 Average	0.0810	
44 Std Dev	0.0006	
45 Rel Std Dev	0.75%	

Charles E. Ed
STABILITY TEST

Operator Signature
CHARLES EDER

Remarks:

Charles Eder

STABILITY TEST

Form 106-I8000

LOT #: 23411080A1

CYL #: 032

Exp. DATE: 10/1/2013

Charles Eder
STABILITY TEST