

INTOXILYZER® 8000 INITIAL INSPECTION

Serial Number: 80-005951

1. Power On and Warm-up:

- a.  Power On
- b.  5 min. Countdown from Initial Warm-up
- c.  1 min. Countdown to Begin a Test
- d.  Forms Load Complete

2. Setup and Checks:

a. Level 1:

- 1) Passwords:  Field Inspector (Level 2)  Lab Personnel (Level 3)
- 2) Gas Cylinder:  Gas Cylinder Setup (Level 1,S)
- 3) Printer:  Printer Setup (Level 3,S,P)  
 Internal Printer Paper Feed  
 Internal Printer Test (Level 1,P)  
 External Printer Test (Level 1,P)
- 4) Barcode Reader (Level 1,B):  Operator ID  
 ND License

b. Level 2:

- 1)  Continuous Purge (Level 2,A)
- 2)  Diagnostic (Level 2,D)
- 3)  Prelim Data Entry (Level 2,E)
- 4)  Ser Num/Version Info (Level 2,V): Ser Num 80-005951  
Version 8164.13

c. Level 3:

- 1) DVM Monitor (Level 3,D,D): 3: 12497 s: 1 C: 47.06  
9: 13111 s: 1 B: 44 0  
(RFI indicator with keyed radio) 1

- 2) Function (F) Keys:  F5 – Tone  
 F6 – Green LED  
 F7 – Red LED  
 F9 – Fan  
 F10 – Pump  
 F11 – Solenoid

- 3) Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 947 CF: 1.06
- 4) Flow Monitor (Level 3,D,F): Flow Sensor, R: 229 F: 0.000 L/s

5) Temperature Monitor (Level 3,D,T): C: 47.0 A: 49.5 I: 0.0

B: 45.0 V: 0.0

6) Tank Monitor (Level 3,D,G): P (gauge): ~225 P (display): 214

7)  General Setup (Level 3,S,G)

8)  Configure Start Test (Level 3,S,T)

9)  Network (Level 3,S,N)

3. Tests:

a. Configure Standard for Wet Bath Simulator (Level 1,S):

1) Zero Alcohol Test (Level 1,C):

Sim Ser #: DR5188 Lot #: MILLI QH<sub>2</sub>O Exp Date: NA

Known Value: 0.000 AC

Results: 0.000 AC 0.000 AC 0.000 AC

2) Low AC Test (Level 1,C):

Sim Ser #: DR3455 Lot #: 12210 Exp Date: 11-2-14

Known Value: 0.020 AC

Results: 0.019 AC 0.019 AC 0.019 AC

3) Linearity Test (Level 1,C):

Sim Ser #: DR3847 Lot #: 13020 Exp Date: 1-15-15

Known Value: 0.300 AC

Results: 0.293 AC 0.295 AC 0.296 AC

b. Configure Dry Gas Standard (Level 1,S):

1) Interferent Detected Tests (Level 1,B):

1. 0.10 AC + 0.05% Acetone

Sim Ser #: DR3377 Lot #: ICS#1 Exp Date: 4-9-14

Known Value: 0.10 AC + 0.05% ACETONE

Display reads "Interferent Detect"

2. Acetone

Sim Ser #: G8919 Lot #: ACE1 Exp Date: 8-27-15

Known Value: 0.05% ACETONE

Display reads "Interferent Detect"

3. Methanol

Sim Ser #: G10573 Lot #: MET1 Exp Date: 8-27-15

Known Value: 0.10% METHANOL

Display reads "Interferent Detect"

4. Isopropanol  
Sim Ser #: G9998 Lot #: IPA1 Exp Date: 8-27-15  
Known Value: 0.10% ISOPROPANOL  
 Display reads "Interferent Detect"
- 2)  Ambient Fail (Level 1,B): Display and test record are correct  
3)  Invalid Sample (Level 1,B): Display and test record are correct  
4)  Subject Test Timeout (Level 1,B): Display and test record are correct.  
5)  Sequence Aborted (Level 1,B): Display and test record are correct  
6)  Control Outside Tolerance (CMS mode): Display and test record are correct  
7)  RFI Detected Test (CMS mode): Display and test record are correct  
8)  Tank Pressure Below Min (CMS mode): Display reads correct  
9)  Subject Refused (CMS mode): Display and test record are correct  
10)  Difference Too Great (CMS mode): Display and test record are correct  
11)  Stability Test (Level 3,T,S):  
Average 0.0809 Std Dev 0.0006 Rel Std Dev 0.73%

Maintenance/Repairs/Notes: \_\_\_\_\_

THIS UNIT IS ACCEPTABLE TO BE USED IN THE FIELD.

  
Field Inspector's Signature

18 SEP 13  
Date

Deb Kashur  
Reviewed by

18 Sept 2013  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-005951  
Location = TOXL 8164.13.00 06/09  
09/17/2013 16:04

\*\*\*\*\* Printer Test \*\*\*\*\*

12 char/line  
abcdefghijkl  
ABCDEFGHIJKL

16 char per line  
abcdefghijklmnop  
ABCDEFGHIJKLMN

21 chars per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

24 characters per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

32 characters per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

42 characters per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

Current Instrument Setup


Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Menfull? Yes  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.080  
Standard Lot #? 23411080A1  
Standard Cyl #? 71  
Standard Expiration? 10/01/2013  
Oper No? 666666

Flow Cal. Date: 06/21/2013  
Slope 693  
Intercept -721277

IR Calibration Date: 06/21/2013

	3um	9um
0th Coef(*100):	-36758	-23512
1st Coef(*100):	274433	137831
2nd Coef(*100):	1462	1190
H2O adj(mg/l*10K):	787	550

\*\*\*\*\* Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks: *INTERNAL  
PRINT  
TEST*  
Form 106-18000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            16:06

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-=  
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-=  
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#%&\*()\_+?

Current Instrument Setup

Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            23411080A1  
Standard Cyl #?            71  
Standard Expiration?        10/01/2013  
Oper No?                    666666

Flow Cal. Date:            06/21/2013  
Slope                        693  
Intercept                    -721277

IR Calibration Date:        06/21/2013

	3um	9um
0th Coef(*100):	-36758	-23512
1st Coef(*100):	274433	137831
2nd Coef(*100):	1462	1190
H2O adj(mg/l*10k):	787	550

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks: *EXTERNAL PRINT  
TEST*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                8164.13.00 06/09  
09/17/2013                        16:10

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *DIAGNOSTIC CHECK*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            16:16

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:16
02 Std. Sol.	0.000	16:17
03 Room Air	0.000	16:18
04 Std. Sol.	0.000	16:18
05 Room Air	0.000	16:19
06 Std. Sol.	0.000	16:20
07 Room Air	0.000	16:20

08 Sim Temp = 34.0°C

Simul Ser No = DR5188  
Std Sol No = MILLIQ H2O  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: ZERO ALCOHOL TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                8164.13.00 06/09  
09/17/2013                        16:25

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:25
02 Std. Sol.	0.019	16:26
03 Room Air	0.000	16:27
04 Std. Sol.	0.019	16:27
05 Room Air	0.000	16:28
06 Std. Sol.	0.019	16:29
07 Room Air	0.000	16:29

08 Sim Temp = 34.0°C

Simul Ser No = DR3455  
Std Sol No = 12210  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *LOW AC TEST*  
*0.020 AC SIM. SOL.*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            16:31

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:32
02 Std. Sol.	0.293	16:32
03 Room Air	0.000	16:33
04 Std. Sol.	0.295	16:34
05 Room Air	0.000	16:34
06 Std. Sol.	0.296	16:35
07 Room Air	0.000	16:35

08 Sim Temp = 34.0°C

Simul Ser No = DR3847  
Std Sol No = 13020  
County = 08                            Oper No. = 666666

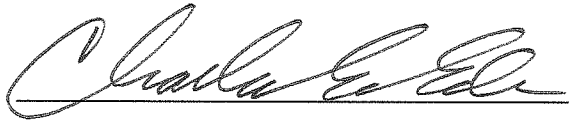

Operator Signature  
CHARLES EDER

Remarks: *LINEARITY TEST*  
*0.300AC Sim. Sol.*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            16:40

Test	AC	Time
01 Room Air	0.000	16:41
02 *Subject Test	INT*	16:42
03 Room Air	0.000	16:43

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = 0.10AC+0.05ACE  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*INTERFERENT  
DETECTED TEST*

Form 106-I8000

*0.10 AC + 0.05% ACETONE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013    16:45

Test	AC	Time
01 Room Air	0.000	16:46
02 *Subject Test	INT*	16:47
03 Room Air	0.000	16:47

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female    Weight = 150  
Test = DUI    Cit = 0.05 ACETONE  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08    Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INTERFERENT  
DETECTED TEST*

Form 106-I8000

*0.05% ACETONE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                8164.13.00 06/09  
09/17/2013                        16:48

Test	AC	Time
01 Room Air	0.000	16:49
02 *Subject Test	INT*	16:50
03 Room Air	0.000	16:50

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = 0.10 METHANOL  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*INTERFERENT DETECTED TEST*  
*0.10% METHANOL*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-005951  
Location = TOXL                                      8164.13.00 06/09  
09/17/2013    16:51

Test	AC	Time
01 Room Air	0.000	16:52
02 *Subject Test	INT*	16:53
03 Room Air	0.000	16:53

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                                      Weight = 150  
Test = DUI    Cit = 0.10 IPA  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08    Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INTERFERENT DETECTED  
TEST*

Form 106-I8000

*0.10% ISOPROPANOL*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            16:55

Test	AC	Time
01 Room Air	AMB*	16:56
02 Room Air	0.000	16:56

\*Invalid Test  
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = AMBIENT FAIL  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: AMBIENT FAIL TEST


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                8164.13.00 06/09  
09/17/2013                                16:57

Test	AC	Time
01 Room Air	0.000	16:58
02 Invalid Sample	X.XXX	16:59
03 Room Air	0.000	17:00

\*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                        Weight = 150  
Test = DUI                                Cit = INVALID SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                                Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INVALID SAMPLE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL            8164.13.00 06/09  
09/17/2013            17:00

Test	AC	Time
01 Room Air	0.000	17:01
02 *Subject Test	0.000*	17:04
03 Room Air	0.000	17:05

No RFI Detected

\*Deficient Sample - Value Printed was  
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female            Weight = 150  
Test = DUI            Cit = TEST TIMEOUT  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *SUBJECT TEST*  
*TIMEOUT*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL            8164.13.00 06/09  
09/17/2013                            17:06

Test	AC	Time
01 Room Air	ABT*	17:07
02 Room Air	0.000	17:07

\*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                    Cit = SEQUENCE ABORT  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                    Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *SEQUENCE ABORTED*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            17:09

Test	AC	Time
01 Diagnostic	OK	17:10
02 Room Air	0.000	17:11
03 Subject Test 1	0.098	17:11
04 Room Air	0.000	17:13
05 Std. Gas	0.088*	17:14
06 Room Air	0.000	17:15

\*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = CON OUT TOL  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *CONTROL OUTSIDE  
OF TOLERANCE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-005951  
Location = TOXL                              8164.13.00 06/09  
09/17/2013    17:15

Test	AC	Time
01 Diagnostic	OK	17:16
02 Room Air	RFI*	17:16
03 Room Air	0.000	17:17

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                              Weight = 150  
Test = DUI                                      Cit = RFI CHECK  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                                      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*RFI CHECK*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            17:18

Test	AC	Time
01 Diagnostic	OK	17:19
02 Room Air	0.000	17:20
03 *Subject Test	REF*	17:20
04 Room Air	0.000	17:20

\*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = SUBJECT REFUSED  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*SUBJECT  
REFUSED*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL            8164.13.00 06/09  
09/17/2013                            17:21

Test	AC	Time
01 Diagnostic	OK	17:21
02 Room Air	0.000	17:22
03 Subject Test 1	0.041*	17:22
04 Room Air	0.000	17:25
05 Std. Gas	0.082	17:26
06 Room Air	0.000	17:27
07 Subject Test 2	0.097*	17:28
08 Room Air	0.000	17:29

\*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                            Weight = 150  
Test = DUI                            Cit = DIFF TOO GREAT  
Dr. Lic. = ND/DIS821456  
Lot No = 23411080A1  
Cyl No = 71  
Expiration Date = 10/01/2013  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

DIFFERENCE TOO  
GREAT

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005951  
Location = TOXL                    8164.13.00 06/09  
09/17/2013                            17:30

Test	AC	Time
01 Room Air	0.000	17:30
02 Std. Gas	0.080	17:31
03 Room Air	0.000	17:31
04 Std. Gas	0.081	17:31
05 Room Air	0.000	17:32
06 Std. Gas	0.080	17:32
07 Room Air	0.000	17:33
08 Std. Gas	0.081	17:33
09 Room Air	0.000	17:34
10 Std. Gas	0.081	17:34
11 Room Air	0.000	17:35
12 Std. Gas	0.081	17:35
13 Room Air	0.000	17:35
14 Std. Gas	0.081	17:36
15 Room Air	0.000	17:36
16 Std. Gas	0.080	17:37
17 Room Air	0.000	17:37
18 Std. Gas	0.081	17:38
19 Room Air	0.000	17:38
20 Std. Gas	0.081	17:38
21 Room Air	0.000	17:39
22 Std. Gas	0.081	17:39
23 Room Air	0.000	17:40
24 Std. Gas	0.081	17:40
25 Room Air	0.000	17:41
26 Std. Gas	0.080	17:41
27 Room Air	0.000	17:42
28 Std. Gas	0.080	17:42
29 Room Air	0.000	17:42
30 Std. Gas	0.082	17:43
31 Room Air	0.000	17:43
32 Std. Gas	0.081	17:44
33 Room Air	0.000	17:44
34 Std. Gas	0.082	17:44
35 Room Air	0.000	17:45
36 Std. Gas	0.081	17:45
37 Room Air	0.000	17:46
38 Std. Gas	0.081	17:46
39 Room Air	0.000	17:47
40 Std. Gas	0.081	17:47
41 Room Air	0.000	17:48
42 Cal Check Stats:		
43 Average	0.0809	
44 Std Dev	0.0006	
45 Rel Std Dev	0.73%	

STABILITY TEST  
Charles E. Ed  
pg 1 of 2

Operator Signature  
CHARLES EDER

Remarks:

STABILITY TEST

Form 106-I8000

Lot#: 23411080A1

Cyl #: 071

Exp. DATE: 10/1/2013

STABILITY TEST  
Charles Eder  
pg 2 of 2