



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Lori Flaten</u>		
Location: <u>MAND</u>		
Intoxilyzer® Serial Number: <u>80-004939</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>40</u>	Expiration Date: <u>09-03-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.080</u> %		
Test 2: <u>0.079</u> %		
Test 3: <u>0.081</u> %		
(ATTACH TEST RECORD)		

Chemical Test Operator Signature

09-24-10
Date

Reviewed By

17 Dec 2010
Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.13.00 06/09
09/24/2010 16:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:43
02 Std. Gas	0.080	16:43
03 Room Air	0.000	16:44
04 Std. Gas	0.079	16:44
05 Room Air	0.000	16:45
06 Std. Gas	0.081	16:45
07 Room Air	0.000	16:46

Lot No = 659358
Cyl No = 40
Exp Date = 09/03/2011
County = 30 Oper No. = 068019

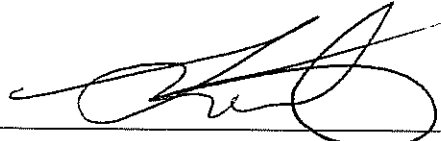

Operator Signature
LORI E. FLATEN

Remarks:

Form 106-18000

80-004939
P. 44 of 44
FLA