



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Johnny Z LAWSON

Location: Bowman Co Sheriff's Dept.

Intoxilyzer Serial No.: 80-004188

Lot Number: 659358

Cylinder Number: 51

Expiration Date: 09/03/2011

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 082 %

Test 2: 0. 082 %

Test 3: 0. 082 %

(ATTACH TEST RECORD)

[Signature]
 Chemical Test Operator Signature

NEW Instrument
 Date Cylinder Changed

Changed 9-30-09 - Noted by map

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-004188
 p. 2 of 2 FW

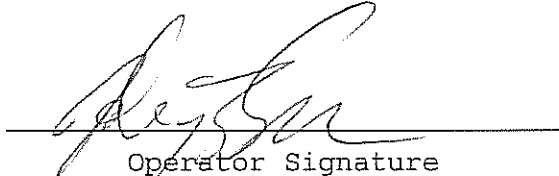
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = BOWM 8164.12.00 06/09
09/30/2009 09:08

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:09
02 Std. Gas	0.082	09:09
03 Room Air	0.000	09:10
04 Std. Gas	0.082	09:10
05 Room Air	0.000	09:11
06 Std. Gas	0.082	09:11
07 Room Air	0.000	09:12

Lot No = 659358
Cyl No = 51
Exp Date = 09/03/2011
County = 06 Oper No. = 020814


Operator Signature
JOHNNY Z. LAWSON

Remarks:

ACA TEST

Form 106-I8000

*80-004188
P. 2 of 2 FR*