



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Jonathan R. Lampi

Location: GFPD

Intoxilyzer Serial No.: 80-003066

Lot Number: 659358

Cylinder Number: 12

Expiration Date: 09-03-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0.081 %

Test 2: 0.082 %

Test 3: 0.082 %

(ATTACH TEST RECORD)

Jonathan R. Lampi, 649
 Chemical Test Operator Signature
Deb Kashner

10-01-09
 Date Cylinder Changed
20 Oct 09

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-003066
 P. 1 of 2
 JRL

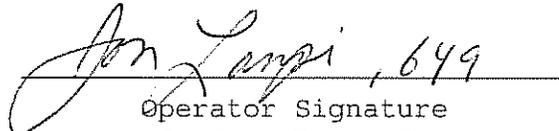
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003066
Location = GFPD 8164.12.00 06/09
10/01/2009 17:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	17:28
02 Std. Gas	0.081	17:29
03 Room Air	0.000	17:29
04 Std. Gas	0.082	17:30
05 Room Air	0.000	17:30
06 Std. Gas	0.082	17:31
07 Room Air	0.000	17:31

Lot No = 659358
Cyl No = 12
Exp Date = 09/03/2011
County = 18 Oper No. = 039947


Operator Signature
JONATHAN R. LAMPI

Remarks:

Cylinder Installation A C A

Form 106-I8000

80-003066
P. 2 of 2
RM