

✓
Database
ann

**INTOXILYZER® 5000 G AND 8000
INSTALLATION AND REPAIR CHECKOUT**

Serial No.: 80-004200 Instrument Location: Cavalier County SO

Reason for Install/Repair: _____ Install After Lab Repair/Inspection
✓ Other (specify) new instrument

Check When Done:

- ✓ A. Surge Protector Installed/Properly Grounded.
- ✓ B. Telephone Line Connected to Intoxilyzer® KB.
- ✓ C. Breath Tube Heated.
- ✓ D. Review/Enter Preliminary Data Entry (Level 2, Function E).
- ✓ E. Ethanol Breath Standard: _____ Connected ✓ Installed.
(Include Form 105-G if New Cylinder Installed.)
- ✓ F. Review/Enter Gas Setup (Level 1, Function S). (Intoxilyzer® 8000 Only.)
- ✓ G. Print Test (Level 1, Function P). (Attach Test Record.)
- ✓ H. ACA Test (Level 1, Function C). (Attach Test Record.)
- ✓ I. RFI Test (Use CMS Mode-First Room Air). (Attach Test Record.)
- J. Repair and/or Maintenance Performed: _____

10/02/2009
Date
13 Oct 09
Date

David J. Zaw
Field Inspector's Signature
Deb Kashner
Reviewed By

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = LANG 8164.12.00 06/09
10/02/2009 14:10

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 659358
Standard Cyl #? 53
Standard Expiration? 05/28/2011
Oper No? 067518

Flow Cal. Date: 06/04/2009
Slope 715
Intercept -655593

IR Calibration Date: 06/03/2009

	3um	9um
0th Coef(*100):	-17852	-24276
1st Coef(*100):	261183	140006
2nd Coef(*100):	2285	945
H2O adj(mg/l*10k):	600	514

***** Printer Test End *****

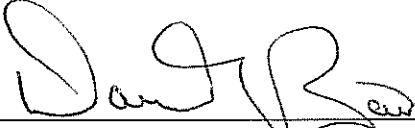
Operator Signature
DAVID J. ZEIS

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = LANG 8164.12.00 06/09
10/02/2009 14:47

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:48
02 Std. Gas	0.082	14:48
03 Room Air	0.000	14:49
04 Std. Gas	0.082	14:49
05 Room Air	0.000	14:50
06 Std. Gas	0.080	14:50
07 Room Air	0.000	14:51

Lot No = 659358
Cyl No = 53
Exp Date = 05/28/2011
County = 10 Oper No. = 067518



Operator Signature
DAVID J. ZEIS

Remarks:

Form 106-I8000

80-004200
P. 3 of 4
JH


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = LANG 8164.12.00 06/09
10/02/2009 14:26

Test	AC	Time
01 Room Air	RFI*	14:28
02 Room Air	0.000	14:28

*Invalid Test
Inhibited - RFI

Sub Name = TEST, SUBJECT NA
Sub DOB = 01/01/2009
Sub Sex = Male Weight = 100
Test = OTH Cit = 1
Dr. Lic. = ND/12
Lot No = 659358
Cyl No = 53
Expiration Date = 05/28/2011
County = 10 Oper No. = 067518

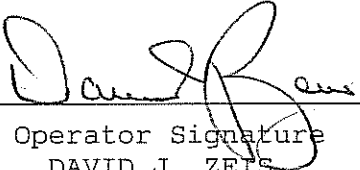

Operator Signature
DAVID J. ZEIS

Remarks:

Form 106-I8000

80-004200
P. 4 of 4 JAL