



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Ronald E. Nord

Location: Walsh LEC, Grafton

Intoxilyzer Serial No.: 80-003072

Lot Number: 659358

Cylinder Number: 16

Expiration Date: 9-3-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 082 %

Test 2: 0. 082 %

Test 3: 0. 050 %

(ATTACH TEST RECORD)

Ronald E. Nord
 Chemical Test Operator Signature

10-07-10 Not changed
 Date Cylinder Changed cylinder checked

Deb Kashur
 Reviewed By

18th Oct 2010
 Date

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-003072
 P. 96 of 97
 KEM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GRAF 8164.13.00 06/09
10/07/2010 18:34

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:35
02 Std. Gas	0.082	18:35
03 Room Air	0.000	18:36
04 Std. Gas	0.082	18:36
05 Room Air	0.000	18:37
06 Std. Gas	0.080	18:37
07 Room Air	0.000	18:37


Lot No = 659358

Cyl No = 16

Exp Date = 09/03/2011

County = 50

Oper No. = 099112

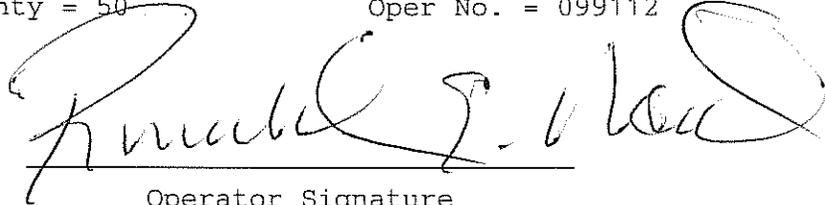

Operator Signature
RONALD E. NORD

Remarks:

Form 106-I8000

80-003072
P. 97 of 97
RAN