



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: John L. Fulwider 068105

Location: WATF

Intoxilyzer Serial No.: 80-004189

Lot Number: 659357

Cylinder Number: 44

Expiration Date: 09/03/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: ^{DK} 0.079 %

Test 2: 0.079 %

Test 3: 0.080 %

(ATTACH TEST RECORD)

John L. Fulwider
 Chemical Test Operator Signature

10-8-09
 Date Cylinder Changed

Deb Kashur
 Reviewed By

06 NOV 09
 Date

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-004189
 P.1 of 2 FN

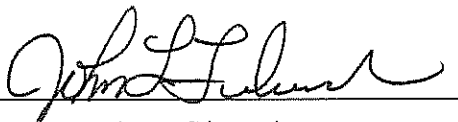
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = WATF 8164.12.00 06/09
10/08/2009 13:45

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:45
02 Std. Gas	0.079	13:46
03 Room Air	0.000	13:46
04 Std. Gas	0.079	13:47
05 Room Air	0.000	13:47
06 Std. Gas	0.080	13:47
07 Room Air	0.000	13:48

Lot No = 659357
Cyl No = 44
Exp Date = 09/03/2011
County = 27 Oper No. = 068105


Operator Signature
JOHN L. FULWIDER

Remarks:

ACA
Setup - Connected Installation
of cylinder

Form 106-I8000

80-004189
P. 2 of 2 JLF