

INTOXILYZER® 5000 G AND 8000  
INSTALLATION AND REPAIR CHECKOUT

Serial No.: 80-004199 Instrument Location: Rolla ✓

Reason for Install/Repair: \_\_\_\_\_ Install After Lab Repair/Inspection  
 Other (specify) New at location

Check When Done:

- A. Surge Protector Installed/Properly Grounded.
- B. Telephone Line Connected to Intoxilyzer® KB.
- C. Breath Tube Heated.
- D. Review/Enter Preliminary Data Entry (Level 2, Function E).
- E. Ethanol Breath Standard:  Connected \_\_\_\_\_ Installed.  
(Include Form 105-G if New Cylinder Installed.)
- F. Review/Enter Gas Setup (Level 1, Function S). (Intoxilyzer® 8000 Only.)
- G. Print Test (Level 1, Function P). (Attach Test Record.)
- H. ACA Test (Level 1, Function C). (Attach Test Record.)
- I. RFI Test (Use CMS Mode-First Room Air). (Attach Test Record.)
- J. Repair and/or Maintenance Performed: \_\_\_\_\_

10-08-09  
Date  
26 Oct 09  
Date

[Signature]  
Field Inspector's Signature  
Deb Kasher  
Reviewed By




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004199  
Location = ROLL      8164.12.00 06/09  
10/08/2009      15:47

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:48
02 Std. Gas	0.078	15:48
03 Room Air	0.000	15:49
04 Std. Gas	0.079	15:49
05 Room Air	0.000	15:49
06 Std. Gas	0.079	15:50
07 Room Air	0.000	15:50

Lot No = 659358  
Cyl No = 11  
Exp Date = 09/03/2011  
County = 40      Oper No. = 010105

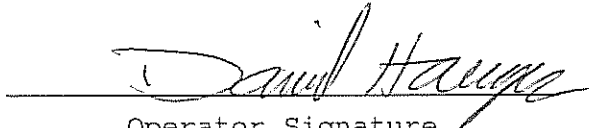  
Operator Signature  
DANIEL J. HAUGEN

Remarks: *ACA at New location*

Form 106-I8000

*80-004199  
P. 3 of 4*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004199  
Location = ROLL      8164.12.00 06/09  
10/08/2009      15:52

Test	AC	Time
01 Diagnostic	OK	15:54
02 Room Air	RFI*	15:54
03 Room Air	0.000	15:55

\*Invalid Test  
Inhibited - RFI

Sub Name = RFI TEST, TEST J  
Sub DOB = 01/01/1989  
Sub Sex = Male      Weight = 200  
Test = DUI      Cit = 111111  
Dr. Lic. = ND/333388888  
Lot No = 659358  
Cyl No = 11  
Expiration Date = 09/03/2011  
County = 40      Oper No. = 010105

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

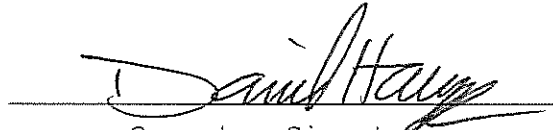

Operator Signature  
DANIEL J. HAUGEN

Remarks:

*RFI at New location*

Form 106-I8000

*80-004199  
P. 7 of 4m*