



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Sgt Brian Crisslen

Location: Belcourt Police Dept

Intoxilyzer Serial No.: ~~86-00377~~ ^{DK} 80-003071 80-003071 CML

Lot Number: 659357

Cylinder Number: 38

Expiration Date: 09/03/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 081 %

Test 2: 0. 081 %

Test 3: 0. 081 %

(ATTACH TEST RECORD)

Sgt Brian Crisslen
 Chemical Test Operator Signature

10-8-09
 Date Cylinder Changed

Dob Kashner
 Reviewed By

16 Oct 09
 Date

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-003071
 P. 1st 2 pm

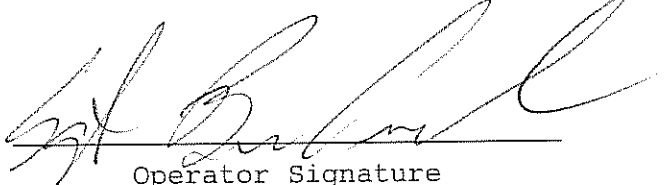
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = BELC 8164.12.00 06/09
10/09/2009 21:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:38
02 Std. Gas	0.081	21:38
03 Room Air	0.000	21:38
04 Std. Gas	0.081	21:39
05 Room Air	0.000	21:39
06 Std. Gas	0.081	21:40
07 Room Air	0.000	21:40

Lot No = 659357
Cyl No = 38
Exp Date = 09/03/2011
County = 63 Oper No. = 119802


Operator Signature
BRIAN F. CRISSLER

Remarks: *New Install*

Form 106-18000

80-003071
P. 2 of 2 km