



OFFICE OF ATTORNEY GENERAL  
 Crime Laboratory Division  
 2641 East Main Avenue  
 P.O. Box 937  
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

**ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM**

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: DOLF A. OLDENBURG

Location: GRAF

Intoxilyzer Serial No.: 80-004193

Lot Number: 659358

Cylinder Number: 16

Expiration Date: 09/03/2011

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. .079 %

Test 2: 0. .079 %

Test 3: 0. .080 %

(ATTACH TEST RECORD)

D. Oldenburg 274 NDHP.  
 Chemical Test Operator Signature

10/09/09  
 Date Cylinder Changed

Deb Kashner  
 Reviewed By

16 Oct 09  
 Date

Form 105-G  
 Toxicology Laboratory  
 Crime Laboratory Division

80-004193  
 p. 1 of 2 rkr

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004193  
Location = GRAF      8164.12.00 06/09  
10/09/2009      09:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:52
02 Std. Gas	0.079	09:52
03 Room Air	0.000	09:53
04 Std. Gas	0.079	09:53
05 Room Air	0.000	09:53
06 Std. Gas	0.080	09:54
07 Room Air	0.000	09:54

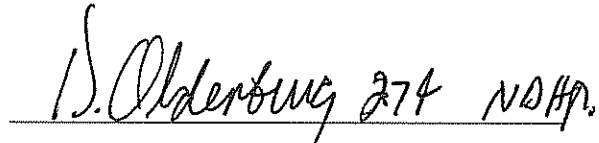
Lot No = 659358

Cyl No = 16

Exp Date = 09/03/2011

County = 50

Oper No. = 048915

  
Operator Signature  
DOLF H. OLDENBURG

Remarks:

Form 106-I8000

80-004193  
P. 2 of 2 FL