



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Aaron R. Hummel</u>		
Location: <u>GFSO</u>		
Intoxilyzer® Serial Number: <u>80-003057</u>		
Gas Lot Number: <u>668180</u>	Gas Cylinder Number: <u>46</u>	Expiration Date: <u>9/21/11</u>
<input checked="" type="checkbox"/> New Cylinder Installed <input type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <del>0.081</del> % <u>0.082</u> DK		
Test 2: <u>0.081</u> %		
Test 3: <u>0.082</u> %		
(ATTACH TEST RECORD)		

[Signature]  
Chemical Test Operator Signature

10/9/10  
Date

Deb Kashner  
Reviewed By

21 Oct 2010  
Date

80-003057  
P. 109-112  
KTM


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003057  
Location = GFSO      8164.13.00 06/09  
10/09/2010      16:50

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:51
02 Std. Gas	0.082	16:51
03 Room Air	0.000	16:52
04 Std. Gas	0.081	16:52
05 Room Air	0.000	16:53
06 Std. Gas	0.082	16:53
07 Room Air	0.000	16:54

Lot No = ~~659357~~ 468180 DK  
Cyl No = ~~26~~ 46  
Exp Date = ~~09/03/2011~~ 9/21/11  
County = 18      Oper No. = 049907

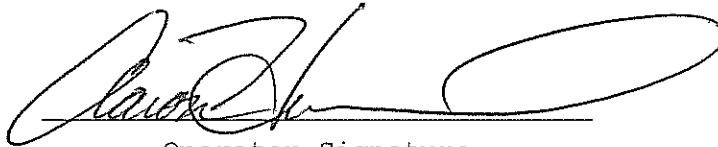

Operator Signature  
AARON HUMMEL

Remarks: *New Cylinder Install*

Form 106-I8000

80-003057  
P. 110 of 112  
JCM



**ETHANOL BREATH STANDARD CYLINDER REPORT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Aaron R. Hummel</u>		
Location: <u>GFSO</u>		
Intoxilyzer@ Serial Number: <u>80-003057</u>		
Gas Lot Number: <u>668180</u>	Gas Cylinder Number: <u>46</u>	Expiration Date: <u>9/21/11</u>
<input checked="" type="checkbox"/> New Cylinder Installed <input type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: <u>0.081</u> % <u>0.082 DK / ARH</u> Test 2: <u>0.081</u> % Test 3: <u>0.082</u> %		

(ATTACH TEST RECORD)

[Signature]  
 Chemical Test Operator Signature

10/9/10  
 Date

Deb Kashur  
 Reviewed By

21 Oct 2010  
 Date


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-003057  
Location = GFSO                    8164.13.00 06/09  
10/09/2010                            16:50

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:51
02 Std. Gas	0.082	16:51
03 Room Air	0.000	16:52
04 Std. Gas	0.081	16:52
05 Room Air	0.000	16:53
06 Std. Gas	0.082	16:53
07 Room Air	0.000	16:54

Lot No = ~~659357~~ 668180 DK/ARK  
Cyl No = ~~2646~~ /ARK  
Exp Date = ~~09/03/2011~~ 9/21/11/ARK  
County = 18                            Oper No. = 049907

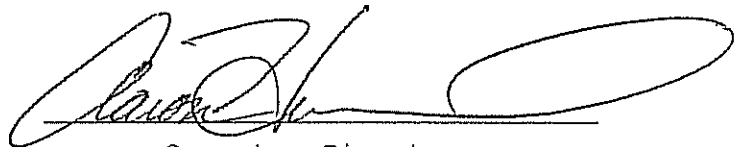

Operator Signature  
AARON HUMMEL

Remarks: *New Cylinder Install*

Form 106-18000

80-003057  
p. 112 of 112  
YR