



# INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59281 (5-2011)

Serial Number	80-004954	Instrument Location	Robette Co (Roka)
Reason for Install/Repair			
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____			

### Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (Use CMS Mode; Key Radio During First Room Air).
- 7. Repair and/or Maintenance Performed (if Any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature	<i>Robert Kennedy</i>	Date	10/16/12
Reviewed By (Crime Laboratory Use Only)	<i>Deb Kashner</i>	Date	21 NOV 12

This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Certified By: *Charles E. Edin* Certified Date: 30 Nov. 2016

Intoxilyzer Test Record and Checklist  
NDCA's Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-004954  
Location = ROLL 8164.13.00 06/09  
10/16/2012 12:32

\*\*\*\*\* Printer Test \*\*\*\*\*

12 char/line  
abcdefghijkl  
ABCDEFGHIJKL

16 char per line  
abcdefghijklmnop  
ABCDEFGHIJKLMN

21 chars per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMNQRSTU

24 characters per line  
abcdefghijklmnopqrstuwx  
ABCDEFGHIJKLMNQRSTUWX

32 characters per line  
abcdefghijklmnopqrstuwx123456  
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line  
abcdefghijklmnopqrstuwx1234567890abccef  
ABCDEFGHIJKLMNQRSTUWXYZ1234567890ABCDEF

Current Instrument Setup


Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Menu!!? No  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.000  
Standard Lot #? 23411080A1  
Standard Cyl #? 61  
Standard Expiration? 10/01/2013  
Oper No? 069108

Flow Cal. Date: 08/27/2012  
Slope 670  
Intercept -570610

IR Calibration Date: 08/27/2012

	Sum	Sum
0th Coef(*100):	-22689	-21316
1st Coef(*100):	260406	132331
2nd Coef(*100):	1084	919
H2O adj(mg/l*10k):	570	470

\*\*\*\*\* Test End \*\*\*\*\*

  
Operator Signature  
ROBERT W. KENNEDY

Remarks:

Form 106-18000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004954  
Location = ROLL      8164.13.00 06/09  
10/16/2012      12:36

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:37
02 Std. Gas	0.081	12:37
03 Room Air	0.000	12:37
04 Std. Gas	0.081	12:38
05 Room Air	0.000	12:38
06 Std. Gas	0.081	12:39
07 Room Air	0.000	12:39

Lot No = 23411080A1  
Cyl No = 61  
Exp Date = 10/01/2013  
County = 40      Oper No. = 069108

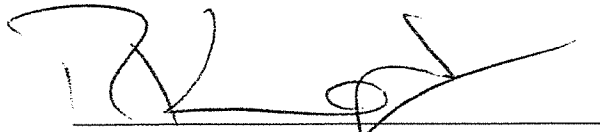

---

Operator Signature  
ROBERT W. KENNEDY

Remarks:

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004954  
Location = ROLL      8164.13.00 06/09  
10/16/2012      12:41

Test	AC	Time
01 Diagnostic	OK	12:42
02 Room Air	RFI*	12:43
03 Room Air	RFI*	12:43

\*Invalid Test  
Inhibited - RFI

Sub Name = RFI, TEST NA  
Sub DOB = 10/16/1999  
Sub Sex = Male      Weight = 123  
Test = DUI      Cit = 9898976  
Dr. Lic. = ND/REF990001  
Lot No = 23411080A1  
Cyl No = 61  
Expiration Date = 10/01/2013  
County = 40      Oper No. = 069108

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

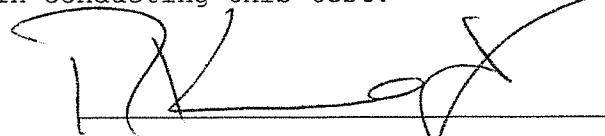

Operator Signature  
ROBERT W. KENNEDY

Remarks: