



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <i>Chad Harmon</i>		
Location <i>FYPD</i>	Intoxilyzer® Serial Number <i>80-004194</i>	
Gas Lot Number <i>33913080A4</i>	Gas Cylinder Number <i>15</i>	Gas Expiration Date <i>01-01-16</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).  
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
  - A. 0. 082 AC
  - B. 0. 082 AC
  - C. 0. 081 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
  - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
  - B. ACA Test Record.

Chemical Test Operator Signature <i>[Signature]</i>	Date <i>10-24-15</i>
Reviewed By (Crime Laboratory Use Only) <i>Deb Shanaver</i>	Date <i>29 Oct 15</i>

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004194  
Location = FYPD      8164.13.00 06/09  
10/24/2015      09:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:30
02 Std. Gas	0.082	09:31
03 Room Air	0.000	09:31
04 Std. Gas	0.082	09:32
05 Room Air	0.000	09:32
06 Std. Gas	0.081	09:33
07 Room Air	0.000	09:33


Lot No = 33913080A4

Cyl No = 15

Exp Date = 01/01/2016

County = 61

Oper No. = 010606

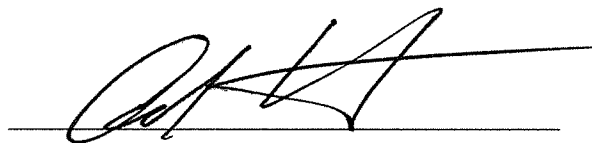

Operator Signature  
CHAD HARMON

Remarks:

Form 106-I8000