



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <i>Sarah Warner</i>		
Location <i>Mott</i>	Intoxilyzer® Serial Number <i>80-004200</i>	
Gas Lot Number <i>16512080A2</i>	Gas Cylinder Number <i>28</i>	Gas Expiration Date <i>08/01/2014</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. 0.081 AC
 - B. 0.080 AC
 - C. 0.080 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Sarah Warner</i>	Date <i>10/25/13</i> ✓
Reviewed By, (Crime Laboratory Use Only) <i>Deb Kashner</i>	Date <i>01 NOV 2013</i>

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = MOTT 8164.13.00 06/09
10/25/2013 13:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:52

*Sequence Aborted

Lot No = 16512080A2
Cyl No = 28
Exp Date = 08/01/2014
County = NA Oper No. = 100620

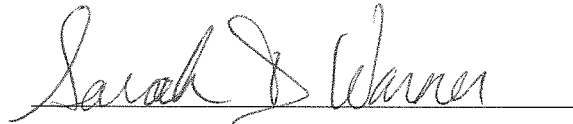

Operator Signature
SARAH WARNER

Remarks: Tried Entering "Hettinger" for County
instead of "21"

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = MOTT 8164.13.00 06/09
10/25/2013 13:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:53

*Sequence Aborted

Lot No = 16512080A2
Cyl No = 28
Exp Date = 08/01/2014
County = NA Oper No. = 100620

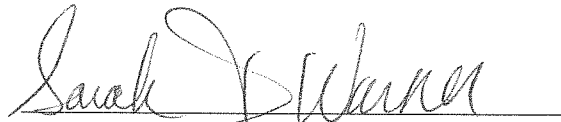

Operator Signature
SARAH WARNER

Remarks: Tried Entering "Hettinger" instead of "21"
for County

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = MOTT 8164.13.00 06/09
10/25/2013 13:54

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:54
02 Std. Gas	0.081	13:55
03 Room Air	0.000	13:55
04 Std. Gas	0.080	13:56
05 Room Air	0.000	13:56
06 Std. Gas	0.080	13:56
07 Room Air	0.000	13:57

Lot No = 16512080A2
Cyl No = 28
Exp Date = 08/01/2014
County = 21 Oper No. = 100620

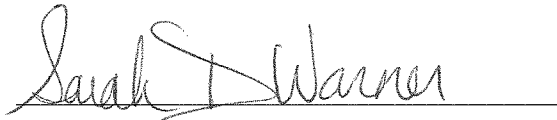
Operator Signature
SARAH WARNER

Remarks:

Form 106-I8000