



ETHANOL GAS STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (10-2013)

Chemical Test Operator Name (Print) Joseph J. Knowski		
Location Rugby Law Enforcement Center		Intoxilyzer® Serial Number 80-004203
Gas Lot Number 16512080A2	Gas Cylinder Number 20	Gas Expiration Date 08/01/2014

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. 0. 083 AC
 - B. 0. 082 AC
 - C. 0. 082 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Joseph J. Knowski</i>	Date 10/26/2013 ✓
Reviewed By (Crime Laboratory Use Only) <i>Deb Kashner</i>	Date 15 NOV 2013

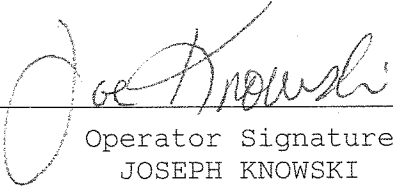
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004203
Location = RUGB 8164.13.00 06/09
10/27/2013 18:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:57
02 Std. Gas	0.083	18:57
03 Room Air	0.000	18:58
04 Std. Gas	0.082	18:58
05 Room Air	0.000	18:59
06 Std. Gas	0.082	18:59
07 Room Air	0.000	19:00

Lot No = 16512080A2
Cyl No = 20
Exp Date = 08/01/2014
County = 35 Oper No. = 109208


Operator Signature
JOSEPH KNOWSKI

Remarks: