



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chad L. Hermon</u>		
Location: <u>FYPD</u>		
Intoxilyzer® Serial Number: <u>80-004954</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>26</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>080</u> %		
Test 2: 0. <u>080</u> %		
Test 3: 0. <u>081</u> %		
(ATTACH TEST RECORD)		

Chad L. Hermon
Chemical Test Operator Signature

11-02-10
Date

Deb Kashner
Reviewed By

08 Nov 2010
Date

80-004954
P. Colafelice

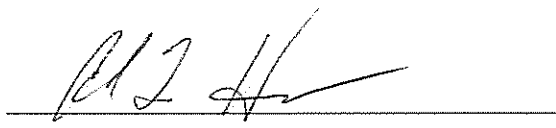
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004954
Location = FYPD 8164.13.00 06/09
11/02/2010 21:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:49
02 Std. Gas	0.080	21:50
03 Room Air	0.000	21:50
04 Std. Gas	0.080	21:50
05 Room Air	0.000	21:51
06 Std. Gas	0.081	21:51
07 Room Air	0.000	21:52

Lot No = 709352
Cyl No = 26
Exp Date = 12/23/2011
County = 61 Oper No. = 010606


Operator Signature
CHAD L. HARMON

Remarks:

Form 106-I8000

80-004954
0.62/62
Ym