



**ETHANOL BREATH STANDARD CYLINDER REPORT**  
OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Hinton, Rick W</u>		
Location: <u>Cass County Jail</u>		
Intoxilyzer® Serial Number: <u>80-004946</u>		
Lot Number: <u>668180</u>	Cylinder Number: <u>76</u>	Expiration Date: <u>9-21-2011</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.76</u> % <u>0.078%</u> <u>DK</u>		
Test 2: <u>0.79</u> %		
Test 3: <u>0.79</u> %		
(ATTACH TEST RECORD)		

[Signature] 3554  
Chemical Test Operator Signature

11/3/10  
Date

Deb Kashner  
Reviewed By

05 NOV 2010  
Date

80-004946  
P. 63 of 64  
1/10/11


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004946  
Location = CASS      8164.13.00 06/09  
11/03/2010      15:39

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:40
02 Std. Gas	0.078	15:41
03 Room Air	0.000	15:41
04 Std. Gas	0.079	15:42
05 Room Air	0.000	15:42
06 Std. Gas	0.079	15:43
07 Room Air	0.000	15:43

Lot No = 668180  
Cyl No = 76  
Exp Date = 09/21/2011  
County = 09      Oper No. = 029920

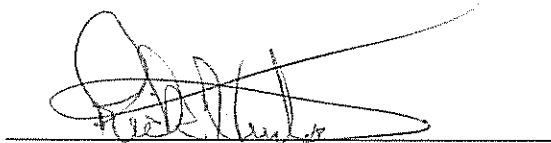

Operator Signature  
RICK HINTON

Remarks:

Form 106-I8000

80-004946  
p. 64 of 64  
JCM