

12/07/2009 13:19 NDOAG - Crime Laboratory Div

(FAX)701 328 6185

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program

Form: BrF-105-G

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Jonathan Lampi

Location: GFPD

Intoxilyzer Serial No.: 80-003062
00 3066 DK

Lot Number: 659358

Cylinder Number: 12

Expiration Date: 09-03-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 080 %

Test 2: 0. 081 %

Test 3: 0. 081 %

(ATTACH TEST RECORD)

Jonathan Lampi
Chemical Test Operator Signature

11-06-09
Date

Deb Kashur
Reviewed By

15 Dec 09
Date

*80-003066
P.1 of 2 FM*

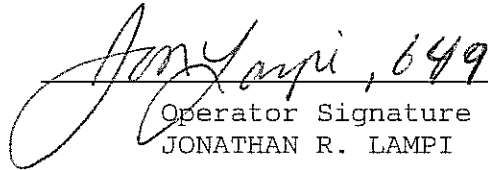
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003066
Location = GFPD 8164.12.00 06/09
11/06/2009 22:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	22:37
02 Std. Gas	0.080	22:38
03 Room Air	0.000	22:38
04 Std. Gas	0.081	22:39
05 Room Air	0.000	22:39
06 Std. Gas	0.081	22:40
07 Room Air	0.000	22:40

Lot No = 659358
Cyl No = 12
Exp Date = 09/03/2011
County = 18 Oper No. = 039947


Operator Signature
JONATHAN R. LAMPI

Remarks:

monthly ACA 120-6

Form 106-I8000

80-003066
p. 2 of 2 FL