



OFFICE OF ATTORNEY GENERAL
Crime Laboratory Division
2641 East Main Avenue
P.O. Box 937
Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: 4. Tracy L. Meidinger #258

Location: UNDP

Intoxilyzer Serial No.: 80-003040

Lot Number: 659358

Cylinder Number: 31

Expiration Date: 09-03-2011

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0.081 %

Test 2: 0.082 %

Test 3: 0.082 %

(ATTACH TEST RECORD)

Tracy L. Meidinger #258
Chemical Test Operator Signature

11-07-2009
Date Cylinder Changed — DK

Deb Kashur
Reviewed By

18 NOV 2009
Date

Form 105-G
Toxicology Laboratory
Crime Laboratory Division

[Type text]

80-003060
p. 1 of 2

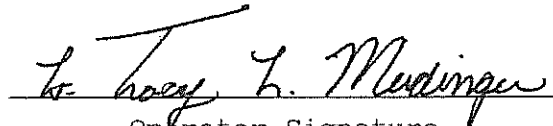
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003060
Location = UNDP 8164.12.00 06/09
11/07/2009 20:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:38
02 Std. Gas	0.081	20:38
03 Room Air	0.000	20:38
04 Std. Gas	0.082	20:39
05 Room Air	0.000	20:39
06 Std. Gas	0.082	20:40
07 Room Air	0.000	20:40

Lot No = 659358
Cyl No = 31
Exp Date = 09/03/2011
County = 18 Oper No. = 119409


Operator Signature
TRACY L. MEIDINGER

Remarks:

Form 106-I8000

ACA Nov 7, 2009

80-003060
P. 2 of 2 SM