



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

DK
ETHANOL BREATH STANDARD CYLINDER-INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Sean Murphy

Location: Bottineau Co. Sheriff's Dept.

Intoxilyzer Serial No.: 80-003067

Lot Number: 659358

Cylinder Number: 55

Expiration Date: 9-3-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 081 %

Test 2: 0. 081 %

Test 3: 0. 082 %

(ATTACH TEST RECORD)

[Signature]
 Chemical Test Operator Signature
Deb Kasher

11-10-09 Tested
 Date Cylinder Changed DK
24 NOV 2009

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-003067
 P. 1 of 2

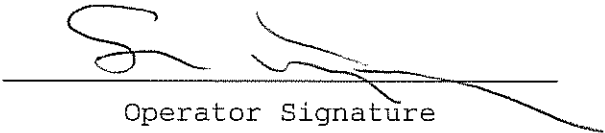
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003067
Location = BOTT 8164.12.00 06/09
11/10/2009 02:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	02:21
02 Std. Gas	0.081	02:22
03 Room Air	0.000	02:22
04 Std. Gas	0.081	02:23
05 Room Air	0.000	02:23
06 Std. Gas	0.082	02:23
07 Room Air	0.000	02:24

Lot No = 659358
Cyl No = 55
Exp Date = 09/03/2011
County = 05 Oper No. = 039117


Operator Signature
SEAN J. MURPHY

Remarks:

Form 106-I8000

80-003067
p. 2 of 2 JM