

OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: DOLF OLDENBURG

Location: GFSD BFKS CB. CORRECTIONAL CENTER

Intoxilyzer Serial No.: 80-003057

Lot Number: 659357

Cylinder Number: 26

Expiration Date: 09/03/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0.081 %

Test 2: 0.081 %

Test 3: 0.081 %

(ATTACH TEST RECORD)

D. Oldenburg 274
 Chemical Test Operator Signature

11/14/09
 Date Cylinder Changed

Deb Kashner
 Reviewed By

04 Dec. 2009
 Date

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003057
Location = GFSO 8164.13.00 06/09
11/14/2009 21:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:56
02 Std. Gas	0.081	21:56
03 Room Air	0.000	21:56
04 Std. Gas	0.081	21:57
05 Room Air	0.000	21:57
06 Std. Gas	0.081	21:58
07 Room Air	0.000	21:58

Lot No = 659357
Cyl No = 26
Exp Date = 09/03/2011
County = 18 Oper No. = 048915

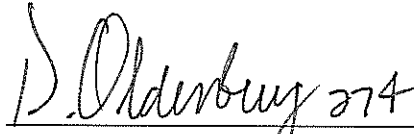

Operator Signature
DOLF OLDENBURG

Remarks:

Form 106-I8000