

11/17/2009 13:22 NDOAG - Crime Laboratory Div



OFFICE OF ATTORNEY GENERAL
Crime Laboratory Division
2641 East Main Avenue
P.O. Box 937
Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Eugene M Molbert

Location: Adams Co SD HETT

Intoxilyzer Serial No.: 80-003072

Lot Number: 659358

Cylinder Number: 7

Expiration Date: 9-03-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 082 %

Test 2: 0. 082 %

Test 3: 0. 083 %

(ATTACH TEST RECORD)

[Signature]
Chemical Test Operator Signature

11-16-09
Date Cylinder Changed DK

Deb Kashner
Reviewed By

18 NOV 2009
Date

Form 105-G
Toxicology Laboratory
Crime Laboratory Division

[Type text]

80-003072
P.1 of 2 FR

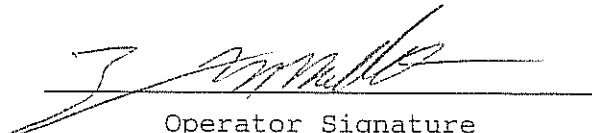
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = HETT 8164.12.00 06/09
11/16/2009 07:33

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	07:34
02 Std. Gas	0.082	07:34
03 Room Air	0.000	07:35
04 Std. Gas	0.082	07:35
05 Room Air	0.000	07:36
06 Std. Gas	0.083	07:36
07 Room Air	0.000	07:37

Lot No = 659358
Cyl No = 7
Exp Date = 09/03/2011
County = 01 Oper No. = 049130


Operator Signature
EUGENE M. MOLBERT

Remarks:

Form 106-I8000

80-003072
P. 2 of 2 FM