



OFFICE OF ATTORNEY GENERAL  
 Crime Laboratory Division  
 2641 East Main Avenue  
 P.O. Box 937  
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER <sup>DK</sup> INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Barry Vannatta

Location: Mob L.

Intoxilyzer Serial No.: 80-004204

Lot Number: 659358

Cylinder Number: 8

Expiration Date: 09-03-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 085 %

Test 2: 0. 085 %

Test 3: 0. 084 %

(ATTACH TEST RECORD)

Barry Vannatta  
 Chemical Test Operator Signature

N/A 11/17/2009 DK  
 Date Cylinder Changed DK

Deb Kashner  
 Reviewed By

18 NOV 2009  
 Date

Form 105-G  
 Toxicology Laboratory  
 Crime Laboratory Division

80-004204  
 P. 1 of 2 FR


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004204  
Location = MOHL      8164.12.00 06/09  
11/17/2009      12:04

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:05
02 Std. Gas	0.085	12:05
03 Room Air	0.000	12:06
04 Std. Gas	0.085	12:06
05 Room Air	0.000	12:07
06 Std. Gas	0.084	12:07
07 Room Air	0.000	12:08

Lot No = 659358  
Cyl No = 8  
Exp Date = 09/03/2011  
County = 38      Oper No. = 039909

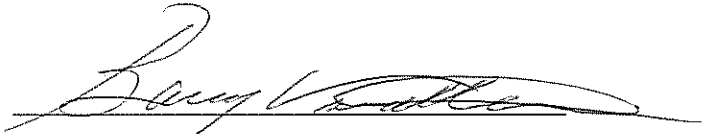

Operator Signature  
BARRY A. VANNATTA

Remarks:

Form 106-I8000

80-004204  
P. 2 of 2 JEM