

12/07/2009 13:33 NDOAG - Crime Laboratory Div

(FAX)701 328 6185

P.002/004

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program

Form: BrF-105-G

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: DAVID J. Zeis

Location: CAVALIER County SO Langdon

Intoxilyzer Serial No.: 80-004200

Lot Number: 659358

Cylinder Number: 53

Expiration Date: 05/28/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 084 %

Test 2: 0. 084 %

Test 3: 0. 084 %

(ATTACH TEST RECORD)

Deb Kashner
Chemical Test Operator Signature

11/20/09
Date

Deb Kashner - ACA
Reviewed By

08 Dec 2009
Date

80-004200
P. 11/20
FM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004200
Location = LANG 8164.12.00 06/09
11/20/2009 08:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:00
02 Std. Gas	0.084	09:00
03 Room Air	0.000	09:01
04 Std. Gas	0.084	09:01
05 Room Air	0.000	09:02
06 Std. Gas	0.084	09:02
07 Room Air	0.000	09:03

Lot No = 659358
Cyl No = 53
Exp Date = 05/28/2011
County = 10 Oper No. = 067518

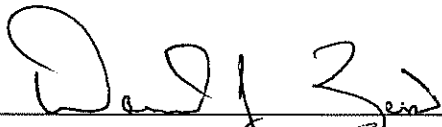

Operator Signature
DAVID J. ZEIS

Remarks:

Form 106-I8000

80-004200
P 2/2
JAN