

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program

Form: BrF-105-G

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Matthew W. Anderson

Location: Richard County Jail

Intoxilyzer Serial No.: 80 004198

Lot Number: 659358

Cylinder Number: 52

Expiration Date: 09/03/2011

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 083 %

Test 2: 0. 082 %

Test 3: 0. 083 %

(ATTACH TEST RECORD)

[Signature]
Chemical Test Operator Signature

12/01/2009
Date

Deb Kashner (ACA)
Reviewed By

08 Dec 2009
Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = WAHP 8164.12.00 06/09
12/01/2009 05:35

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 05:36 |
| 02 Std. Gas | 0.083 | 05:36 |
| 03 Room Air | 0.000 | 05:37 |
| 04 Std. Gas | 0.082 | 05:37 |
| 05 Room Air | 0.000 | 05:38 |
| 06 Std. Gas | 0.083 | 05:38 |
| 07 Room Air | 0.000 | 05:39 |

Lot No = 659358
Cyl No = 52
Exp Date = 09/03/2011
County = 39 Oper No. = 020401

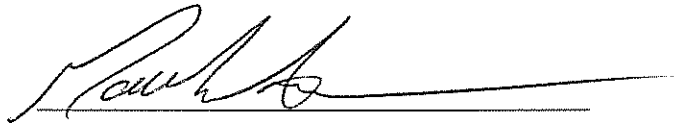

Operator Signature
MATTHEW W. ANDERSON

Remarks: