

OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 Instrument Certification and Maintenance Unit

BrF-005-8

Q. Flow Monitor. Level 3 Func D Sub F. R 159 F 0.000 L/s
 R. Temperature Monitor. Level 3 Func D Sub T
 C 47.0 A 49.0 I 0.0
 B 45.0 V 0.0
 S. Gas Tank Monitor. Level 3 Func D Sub G 1001 psi Intox 1000 psi Reg
 T. Configure Wet Bath Sim. Level 1 Func S
 U. Zero Alcohol Test Level 1 Func C
G10329 Sim SN — Lot 0.000 Rep Value
0.000 AC 87000 AC 0.000 AC
 V. Low AC Test. Level 1 Func C
DR5190 Sim SN — Lot 0.021 Rep Value
0.020 AC 0019 AC 0.019 AC
 W. Linearity Test. Level 1 Func C
DR5113 Sim SN — Lot 0.285 Rep Value
0.295 AC 0.298 AC 0.298 AC
 X. Interferent Test.
 Level 1 Func B
 Acetone DR5186 Sim SN — Lot 0.05% Conc
 Display Printout
 Methanol DR3846 Sim SN — Lot 0.10% Conc
 Display Printout
 IPA DR3840 Sim SN — Lot 0.10% Conc
 Display Printout
 Y. Ambient Test
 Z. Invalid Sample Test
 AA. RFI Detector Test. CMS Mode
 Display Printout
 BB. Configure Dry Gas Standard. Level 1 Func S
 CC. Stability Test at 0.080AC. Level 3 Func T Sub S
0.813 Ave. 0.005 Std Dev 0.58 Rel Std Dev
 DD. Maintenance/Repairs Software 8164.13

MAD
32 December 2009
 Date
08 Dec 2009
 Date

Mary Blain
 Signature
Deb Kashner
 Reviewed by

08/09

80-003059
 P. 2 of 17
 JAH

Intoxilyzer Test Record and Checklist
NDDAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 09:15

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQRSTUWX

32 characters per line
abcdefghijklmnopqrstuwx123456
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuwx1234567890abcdef
ABCDEFGHIJKLMNQRSTUWXYZ1234567890ABCDEF

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Manfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 659357
Standard Cyl #? 37
Standard Expiration? 09/03/2011
Oper No? 107501

Flow Cal. Date: 04/07/2008
Slope: 713
Intercept: -692349

IR Calibration Date: 06/04/2008

| | Sum | Sum |
|--------------------|--------|--------|
| 0th Coef(*100): | -15808 | -12563 |
| 1st Coef(*100): | 279401 | 139560 |
| 2nd Coef(*100): | 1046 | 760 |
| H2O adj(ng/l*10K): | 478 | 208 |

***** Test End *****


Operator Signature
MARGY PEARSON

Remarks:

Form 106-18000

80-003059
P. 3 of 17
JCM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 09:23

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 659357
Standard Cyl #? 37
Standard Expiration? 09/03/2011
Oper No? 107501

Flow Cal. Date: 04/07/2008
Slope 713
Intercept -692349

IR Calibration Date: 06/04/2008
 3um 9um

0th Coef(*100): -15808 -12583
1st Coef(*100): 279401 139580
2nd Coef(*100): 1046 760
H2O adj(mg/l*10k): 478 208

***** Printer Test End *****



Operator Signature
MARGY PEARSON

Remarks:

Print


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 09:46

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 09:48 |
| 02 *Subject Test | REF* | 09:48 |
| 03 Room Air | 0.000 | 09:48 |

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 659358
Cyl No = 34
Expiration Date = 09/03/2011
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:



Form 106-I8000

80-003059
P. 5-17 YH

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 09:25

DIAGNOSTIC

| | |
|---------------------------|------|
| Voltage/Current Test | Pass |
| RAM Test | Pass |
| EEPROM Checksum Test | Pass |
| Real Time Clock Test | Pass |
| DSP Test | Pass |
| Analytical Stability Test | Pass |
| Modem Test | Pass |
| Temp Regulation Test | Pass |

Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Diagnostics

Form 106-I8000

80-003059
P. 6 of 17 yth

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 10:28

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 10:29 |
| 02 Std. Sol. | 0.000 | 10:30 |
| 03 Room Air | 0.000 | 10:30 |
| 04 Std. Sol. | 0.000 | 10:31 |
| 05 Room Air | 0.000 | 10:32 |
| 06 Std. Sol. | 0.000 | 10:32 |
| 07 Room Air | 0.000 | 10:33 |

08 Sim Temp = 34.0°C

Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501


Operator Signature
MARGY PEARSON

Remarks:

0.000 AC Water

Form 106-I8000

80-003059
P. 7 of 17 10/2

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 10:34

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 10:34 |
| 02 Std. Sol. | 0.020 | 10:35 |
| 03 Room Air | 0.000 | 10:36 |
| 04 Std. Sol. | 0.019 | 10:37 |
| 05 Room Air | 0.000 | 10:37 |
| 06 Std. Sol. | 0.019 | 10:38 |
| 07 Room Air | 0.000 | 10:38 |

08 Sim Temp = 34.0°C

Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks: *Low AC 0.021 AC*

Form 106-I8000

*80-003059
P. Def 17 PM*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 10:42

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 10:43 |
| 02 Std. Sol. | 0.295 | 10:54 |
| 03 Room Air | 0.000 | 10:55 |
| 04 Std. Sol. | 0.298 | 10:56 |
| 05 Room Air | 0.000 | 10:56 |
| 06 Std. Sol. | 0.298 | 10:57 |
| 07 Room Air | 0.000 | 10:58 |

08 Sim Temp = 34.0°C

Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Linearity 0.285 AC

Form 106-I8000

*80-003059
P. 9/17/09*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 11:07

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 11:08 |
| 02 *Subject Test | INT* | 11:09 |
| 03 Room Air | 0.000 | 11:09 |

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

0.05% ACETONE - INTERFER

Form 106-I8000

80-003059
P. 10 of 17 JFH


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 11:12

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 11:13 |
| 02 *Subject Test | INT* | 11:13 |
| 03 Room Air | 0.000 | 11:14 |

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

MeOH 0.10% Interfer

Form 106-I8000

80-003059
P.11417A


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 11:10

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 11:11 |
| 02 *Subject Test | INT* | 11:11 |
| 03 Room Air | 0.000 | 11:12 |

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

1 PA 0.10% INTERFER

Form 106-I8000

80-003059
P. 12 of 17 YR


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 12:01

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | AMB* | 12:02 |
| 02 Room Air | 0.000 | 12:03 |

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 659358
Cyl No = 34
Expiration Date = 09/03/2011
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

AMBIENT FAIL

Form 106-I8000

80-003059
P. 13 of 17
JCH


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 12:06

| Test | AC | Time |
|-------------------|-------|-------|
| 01 Room Air | 0.000 | 12:07 |
| 02 Invalid Sample | X.XXX | 12:07 |
| 03 Room Air | 0.000 | 12:08 |

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 659358
Cyl No = 34
Expiration Date = 09/03/2011
County = 08 Oper No. = 107501

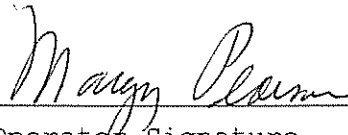

Operator Signature
MARGY PEARSON

Remarks:

Invalid Sample

Form 106-I8000

80-003059
P.14-17
JCH

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 10:58

| Test | AC | Time |
|---------------|-------|-------|
| 01 Diagnostic | OK | 10:59 |
| 02 Room Air | RFI* | 10:59 |
| 03 Room Air | 0.000 | 11:00 |

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 0000000
Std Sol No = 000000
County = 08 Oper No. = 107501

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
MARGY PEARSON

Remarks:

RFI Detect

Form 106-I8000

*80-003059
P. 15-17 jsh*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003059
Location = TOXL 8164.13.00 06/09
12/03/2009 09:49

| Test | AC | Time |
|---------------------|--------|-------|
| 01 Room Air | 0.000 | 09:50 |
| 02 Std. Gas | 0.081 | 09:50 |
| 03 Room Air | 0.000 | 09:51 |
| 04 Std. Gas | 0.082 | 09:51 |
| 05 Room Air | 0.000 | 09:52 |
| 06 Std. Gas | 0.082 | 09:52 |
| 07 Room Air | 0.000 | 09:53 |
| 08 Std. Gas | 0.081 | 09:53 |
| 09 Room Air | 0.000 | 09:54 |
| 10 Std. Gas | 0.081 | 09:54 |
| 11 Room Air | 0.000 | 09:55 |
| 12 Std. Gas | 0.081 | 09:55 |
| 13 Room Air | 0.000 | 09:56 |
| 14 Std. Gas | 0.081 | 09:56 |
| 15 Room Air | 0.000 | 09:57 |
| 16 Std. Gas | 0.081 | 09:57 |
| 17 Room Air | 0.000 | 09:57 |
| 18 Std. Gas | 0.081 | 09:58 |
| 19 Room Air | 0.000 | 09:58 |
| 20 Std. Gas | 0.081 | 09:59 |
| 21 Room Air | 0.000 | 09:59 |
| 22 Std. Gas | 0.081 | 10:00 |
| 23 Room Air | 0.000 | 10:00 |
| 24 Std. Gas | 0.082 | 10:01 |
| 25 Room Air | 0.000 | 10:01 |
| 26 Std. Gas | 0.081 | 10:02 |
| 27 Room Air | 0.000 | 10:02 |
| 28 Std. Gas | 0.081 | 10:03 |
| 29 Room Air | 0.000 | 10:03 |
| 30 Std. Gas | 0.081 | 10:04 |
| 31 Room Air | 0.000 | 10:04 |
| 32 Std. Gas | 0.081 | 10:04 |
| 33 Room Air | 0.000 | 10:05 |
| 34 Std. Gas | 0.082 | 10:05 |
| 35 Room Air | 0.000 | 10:06 |
| 36 Std. Gas | 0.082 | 10:06 |
| 37 Room Air | 0.000 | 10:07 |
| 38 Std. Gas | 0.082 | 10:07 |
| 39 Room Air | 0.000 | 10:08 |
| 40 Std. Gas | 0.081 | 10:08 |
| 41 Room Air | 0.000 | 10:09 |
| 42 Cal Check Stats: | | |
| 43 Average | 0.0813 | |
| 44 Std Dev | 0.0005 | |
| 45 Rel Std Dev | 0.58% | |

*Stability Test
page 1 of 2
MAR*

*80-003059
P. 16 of 17 1/12*

Operator Signature
MARGY PEARSON

Remarks:

LOT# 659358 Cyl 34 Exp 3 Sept 2011

Form 106-I8000

Stability Test
2002
MAP

80-003059
P. 17/17 KM