

**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**

Serial No.: 80-003060 Instrument Location: Mercer Co SO - Stanton

Reason for Install/Repair: \_\_\_\_\_ Install After Lab Repair/Inspection  
X Other (Specify) New machine

Check When Done:

- A. Surge Protector Installed/Properly Grounded.
- B. Telephone Line Connected to Intoxilyzer®.
- C. Breath Tube Heated.
- D. Review/Enter Preliminary Data Entry (Level 2, Function E).
- E. Review/Enter Gas Setup (Level 1, Function S).
- F. Print Test (Level 1, Function P). (Attach Test Record.)
- G. ACA Test (Level 1, Function C). (Attach Test Record.)
- H. RFI Test (Use CMS Mode-First Room Air). (Attach Test Record.)

I. Repair and/or Maintenance Performed: Installed

new Intoxilyzer 8000 to replace 8000 that was not working properly

12/05/2009  
Date

  
Field Inspector's Signature

07 Dec 09  
Date

Deb Kashner  
Reviewed By




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003060  
Location = STAT      8164.13.00 06/09  
12/05/2009      16:35

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:35
02 Std. Gas	0.081	16:36
03 Room Air	0.000	16:36
04 Std. Gas	0.081	16:37
05 Room Air	0.000	16:37
06 Std. Gas	0.082	16:38
07 Room Air	0.000	16:38

Lot No = 659357  
Cyl No = 43  
Exp Date = 09/03/2011  
County = 29      Oper No. = 049121

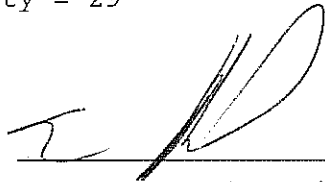

Operator Signature  
NORMAN C. RUUD

Remarks:

Form 106-I8000

80-003060  
P. 3 of 4  
FR


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003060  
Location = STAT      8164.13.00 06/09  
12/05/2009      16:39

Test	AC	Time
01 Diagnostic	OK	16:40
02 Room Air	RFI*	16:41
03 Room Air	0.000	16:41

\*Invalid Test  
Inhibited - RFI

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

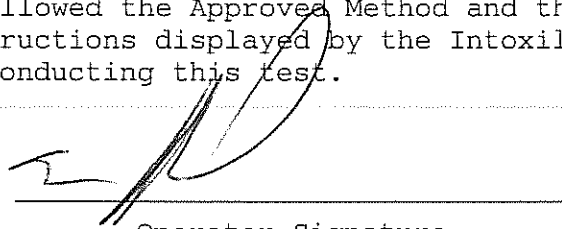

Operator Signature  
NORMAN C. RUUD

Remarks:

Form 106-I8000

80-003060  
P. 4 of 4 JRM