



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name:	Jamie M Huschka				
Location:	Williston LEC				
Intoxilyzer® Serial Number:	80-004189				
Gas Lot Number:	15410020A1	Gas Cylinder Number:	6	Expiration Date:	07/01/12
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed				
Instrument Test Results (Report to 3 Digits; Example, 0.081%)					
Test 1: 0.076 %					
Test 2: 0.077 %					
Test 3: 0.076 %					
(ATTACH TEST RECORD)					

Jamie M Huschka
Chemical Test Operator Signature

5 Dec 2010
Date

Deb Kashner
Reviewed By

27 Dec 2010
Date

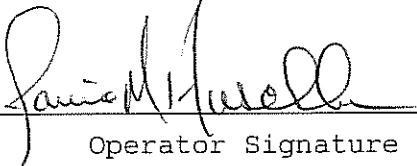
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004189
Location = WILL 8164.13.00 06/09
12/05/2010 18:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:22
02 Std. Gas	0.076	18:22
03 Room Air	0.000	18:23
04 Std. Gas	0.077	18:23
05 Room Air	0.000	18:24
06 Std. Gas	0.076	18:24
07 Room Air	0.000	18:25

Lot No = ~~659357~~ 1541008A1 Dk per Jamie Huschka
Cyl No = ~~45~~ 6 27 Dec 2010
Exp Date = ~~09/03/2011~~ 07/01/12
County = 53 Oper No. = 100406


Operator Signature
JAMIE M. HUSCHKA

Remarks:

Form 106-18000

80-004189
P. 90 of 90
FM