



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Adam Krabbenhoft</u>		
Location: <u>LaMoure County Courthouse</u>		
Intoxilyzer® Serial Number: <u>80-004942</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>14</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>081</u> %		
Test 2: 0. <u>081</u> %		
Test 3: 0. <u>082</u> %		
(ATTACH TEST RECORD)		

[Signature]
Chemical Test Operator Signature

12-7-10
Date

Deb Kashur
Reviewed By

10 Dec '10
Date

80-004942
P. 55 of 56
jan


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004942
Location = LAMO 8164.13.00 06/09
12/07/2010 13:12

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:13
02 Std. Gas	0.081	13:13
03 Room Air	0.000	13:14
04 Std. Gas	0.081	13:14
05 Room Air	0.000	13:15
06 Std. Gas	0.082	13:15
07 Room Air	0.000	13:15

Lot No = 709352
Cyl No = 14
Exp Date = 12/23/2011
County = 23 Oper No. = 020828

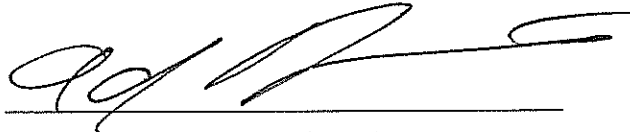

Operator Signature
ADAM R. KRABBENHOFT

Remarks:

ACA Test

Form 106-I8000

80-004942
P. 56 of 56
JSM