



ETHANOL BREATH STANDARD CYLINDER REPORT
OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Hinton, Rick W</u>		
Location: <u>Cass County Jail</u>		
Intoxilyzer® Serial Number: <u>8000 80-004946</u>		
Lot Number: <u>668180</u>	Cylinder Number: <u>76</u>	Expiration Date: <u>9-21-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>79</u> %		
Test 2: 0. <u>79</u> %		
Test 3: 0. <u>79</u> %		
(ATTACH TEST RECORD)		

Rick W Hinton 3554
Chemical Test Operator Signature

12-7-10
Date

Deb Kashner
Reviewed By

10 Dec '10
Date

80-004946
f.65af26
EM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004946
Location = CASS 8164.13.00 06/09
12/07/2010 13:33

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:34
02 Std. Gas	0.079	13:35
03 Room Air	0.000	13:35
04 Std. Gas	0.079	13:35
05 Room Air	0.000	13:36
06 Std. Gas	0.079	13:36
07 Room Air	0.000	13:37

Lot No = 668180
Cyl No = 76
Exp Date = 09/21/2011
County = 09 Oper No. = 029920

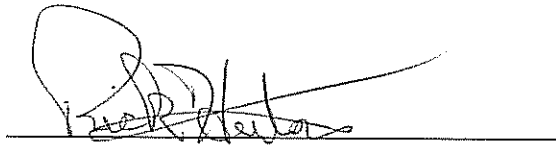

Operator Signature
RICK HINTON

Remarks:

Form 106-I8000

80-064946
P. 46 of 66
sam