

INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

Serial No.: 80004193 Instrument Location: Devils lake LEC.

Reason for Install/Repair: X Install After Lab Repair/Inspection
Other (Specify) _____

Check When Done:

- X A. Surge Protector Installed/Properly Grounded.
- X B. Telephone Line Connected to Intoxilyzer®.
- X C. Breath Tube Heated.
- X D. Review/Enter Preliminary Data Entry (Level 2, Function E).
- X E. Review/Enter Gas Setup (Level 1, Function S).
- X F. Print Test (Level 1, Function P). (Attach Test Record.)
- X G. ACA Test (Level 1, Function C). (Attach Test Record.)
- X H. RFI Test (Use CMS Mode-First Room Air). (Attach Test Record.)
- I. Repair and/or Maintenance Performed: _____

12-10-09.
Date

Joe Knowles
Field Inspector's Signature

30 Dec 2009
Date

Deb Kashur
Reviewed By

80-004193
P. 1 of 4 km

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = DEVL 8164.13.00 06/09
12/10/2009 20:07

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=_|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup

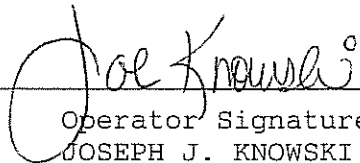
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 659358
Standard Cyl #? 20
Standard Expiration? 09/03/2011
Oper No? 109208

Flow Cal. Date: 06/04/2009
Slope 692
Intercept -611138

IR Calibration Date: 06/03/2009
 3um 9um

0th Coef(*100):	-12132	-15777
1st Coef(*100):	261160	129907
2nd Coef(*100):	1958	971
H2O adj(mg/l*10k):	413	335

***** Printer Test End *****


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

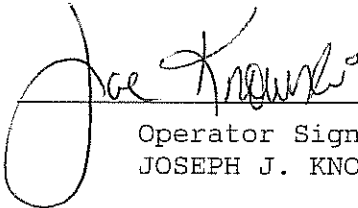
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = DEVL 8164.13.00 06/09
12/10/2009 20:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:11
02 Std. Gas	0.081	20:11
03 Room Air	0.000	20:12
04 Std. Gas	0.082	20:12
05 Room Air	0.000	20:13
06 Std. Gas	0.081	20:13
07 Room Air	0.000	20:14

Lot No = 659358
Cyl No = 20
Exp Date = 09/03/2011
County = 36 Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004193
P. 3 of 4 pages

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

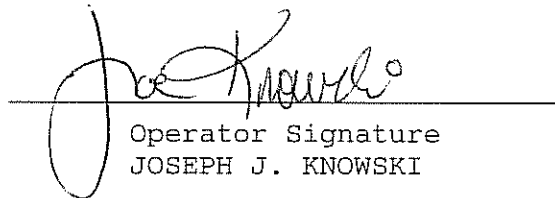
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = DEVL 8164.13.00 06/09
12/10/2009 20:14

Test	AC	Time
01 Diagnostic	OK	20:16
02 Room Air	RFI*	20:16
03 Room Air	0.000	20:16

*Invalid Test
 Inhibited - RFI

Sub Name = JOHNSON, DAVE R
Sub DOB = 12/31/1965
Sub Sex = Male Weight = 123
Test = DUI Cit = 12345
Dr. Lic. = ND/JOH651234
Lot No = 659358
Cyl No = 20
Expiration Date = 09/03/2011
County = 36 Oper No. = 109208

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004193
P. 4 of 4 JJK