

INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

Serial No.: 659357 Instrument Location: Belcourt PD.

Reason for Install/Repair: Install After Lab Repair/Inspection
 Other (Specify) _____

Check When Done:

- A. Surge Protector Installed/Properly Grounded.
- B. Telephone Line Connected to Intoxilyzer®.
- C. Breath Tube Heated.
- D. Review/Enter Preliminary Data Entry (Level 2, Function E).
- E. Review/Enter Gas Setup (Level 1, Function S).
- F. Print Test (Level 1, Function P). (Attach Test Record.)
- G. ACA Test (Level 1, Function C). (Attach Test Record.)
- H. RFI Test (Use CMS Mode-First Room Air). (Attach Test Record.)
- I. Repair and/or Maintenance Performed: _____

12-10-2009.
Date

Joseph Knowlton
Field Inspector's Signature

30 Dec 2009
Date

Deb Kashner
Reviewed By

80-004197
P. 1 of 4
KM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004197
Location = BELC 8164.13.00 06/09
12/10/2009 17:40

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup

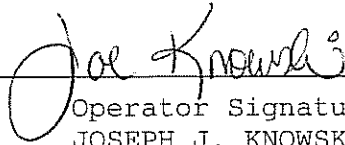
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 659357
Standard Cyl #? 38
Standard Expiration? 09/03/2011
Oper No? 109208

Flow Cal. Date: 06/04/2009
Slope 697
Intercept -597078

IR Calibration Date: 06/03/2009

	3um	9um
0th Coef(*100):	-18382	-32622
1st Coef(*100):	278299	134602
2nd Coef(*100):	929	921
H2O adj(mg/l*10k):	352	627

***** Printer Test End *****


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

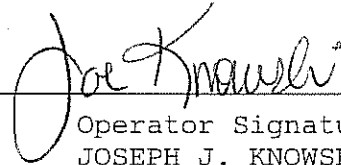
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004197
Location = BELC 8164.13.00 06/09
12/10/2009 17:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	17:47
02 Std. Gas	0.083	17:48
03 Room Air	0.000	17:48
04 Std. Gas	0.083	17:48
05 Room Air	0.000	17:49
06 Std. Gas	0.083	17:49
07 Room Air	0.000	17:50

Lot No = 659357
Cyl No = 38
Exp Date = 09/03/2011
County = 40 Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004197
P. 3 of 4
JKM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004197
Location = BELC 8164.13.00 06/09
12/10/2009 17:51

Test	AC	Time
01 Diagnostic	OK	17:52
02 Room Air	RFI*	17:52
03 Room Air	0.000	17:53

*Invalid Test
Inhibited - RFI

Sub Name = JOHNSON, STEVE K
Sub DOB = 12/31/1965
Sub Sex = Male Weight = 123
Test = DUI Cit = 12345
Dr. Lic. = ND/JOH651234
Lot No = 659357
Cyl No = 38
Expiration Date = 09/03/2011
County = 40 Oper No. = 109208

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80004197
P. 4 of 4
YAK