

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Joe Knowski

Location: Belcourt PD.

Intoxilyzer Serial No.: 80-004197

Lot Number: 659357

Cylinder Number: 38

Expiration Date: 9-3-2009

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 083 %

Test 2: 0. 081 %

Test 3: 0. 082 %

(ATTACH TEST RECORD)

Joe Knowski
Chemical Test Operator Signature

12-10-2009
Date

Deb Kashur
Reviewed By

30 Dec 2009
Date

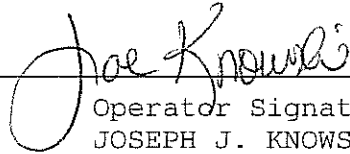
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004197
Location = BELC 8164.13.00 06/09
12/10/2009 17:41

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	17:42
02 Std. Gas	0.083	17:43
03 Room Air	0.000	17:43
04 Std. Gas	0.081	17:43
05 Room Air	0.000	17:44
06 Std. Gas	0.082	17:44
07 Room Air	0.000	17:45

Lot No = 659357
Cyl No = 38
Exp Date = 09/03/2011
County = 40 Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004197
P. 2 of 2
YH