

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Sgt. Joe Knowski

Location: Rolla S.O.

Intoxilyzer Serial No.: 80-004199

Lot Number: 659358

Cylinder Number: 11

Expiration Date: 9-3-2011

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0.082 %

Test 2: 0.081 %

Test 3: 0.082 %

(ATTACH TEST RECORD)

Joseph Knowski
Chemical Test Operator Signature

12-10-2009
Date

Deb Kasher
Reviewed By

30 Dec 2009
Date

80-004199
p. 1 of 2
JK

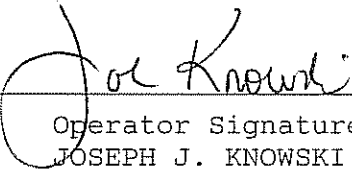
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004199
Location = ROLL 8164.13.00 06/09
12/10/2009 16:04

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:05
02 Std. Gas	0.082	16:05
03 Room Air	0.000	16:06
04 Std. Gas	0.081	16:06
05 Room Air	0.000	16:07
06 Std. Gas	0.082	16:07
07 Room Air	0.000	16:08

Lot No = 659358
Cyl No = 11
Exp Date = 09/03/2011
County = 40 Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004199
P. 2 of 2 JAK