



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Richard D. Johnson</u>		
Location: <u>McLean LEC Washburn ND</u>		
Intoxilyzer® Serial Number: <u>80-004196</u>		
Gas Lot Number: <u>659357</u>	Gas Cylinder Number: <u>47</u>	Expiration Date: <u>9/3/11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: <u>0.081</u> % Test 2: <u>0.080</u> % Test 3: <u>0.080</u> %		
(ATTACH TEST RECORD)		

Richard D. Johnson
 Chemical Test Operator Signature

12-14-10
 Date

Deb Kasher
 Reviewed By

17 Dec 2010
 Date

80-004196
 p. 97 of 98
 sam

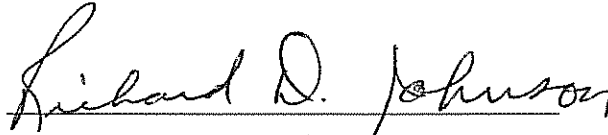
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = WASH 8164.13.00 06/09
12/14/2010 10:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:57
02 Std. Gas	0.081	10:58
03 Room Air	0.000	10:58
04 Std. Gas	0.080	10:59
05 Room Air	0.000	10:59
06 Std. Gas	0.080	11:00
07 Room Air	0.000	11:00

Lot No = 659357
Cyl No = 47
Exp Date = 09/03/2011
County = 28 Oper No. = 118707


Operator Signature
RICHARD D. JOHNSON

Remarks:

Form 106-18000

80-004196
P. 98 of 98
FM