



ETHANOL BREATH STANDARD CYLINDER REPORT  
OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Jacquie DeMaree</u>		
Location: <u>FTT to Hen PD</u>		
Intoxilyzer® Serial Number: <u>80-00494</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>56</u>	Expiration Date: <u>9/23/2011</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.078</u> %		
Test 2: <u>0.077</u> %		
Test 3: <u>0.077</u> %		
(ATTACH TEST RECORD)		

Jacquie DeMaree  
Chemical Test Operator Signature

12-18-09  
Date

Deb Kashur  
Reviewed By

23 Mar 2010  
Date

80-004194  
P. 1 of 2 rsm

7/6/10

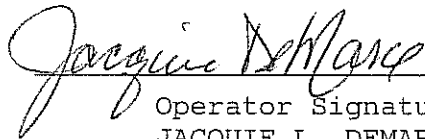
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004194  
Location = FTOT      8164.13.00 06/09  
12/18/2009      15:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:49
02 Std. Gas	0.078	15:49
03 Room Air	0.000	15:50
04 Std. Gas	0.077	15:50
05 Room Air	0.000	15:50
06 Std. Gas	0.077	15:51
07 Room Air	0.000	15:51

Lot No = 659358  
Cyl No = 56  
Exp Date = 09/03/2011  
County = 03      Oper No. = 100103

  
Operator Signature  
JACQUIE L. DEMARCE

Remarks:

Form 106-I8000

80-004194  
P. 20/2 JLM  
77/77