

### ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Jacquie DeMarce

Location: Fort Totten PD

Intoxilyzer Serial No.: 80-004194

Lot Number: 659358

Cylinder Number: 56

Expiration Date: 9-3-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 076%

Test 2: 0. 077 %

Test 3: 0. 077 %

(ATTACH TEST RECORD)

Jacquie DeMarce  
Chemical Test Operator Signature

12-18-09  
Date

Deb Kashur  
Reviewed By

30 Dec 2009  
Date

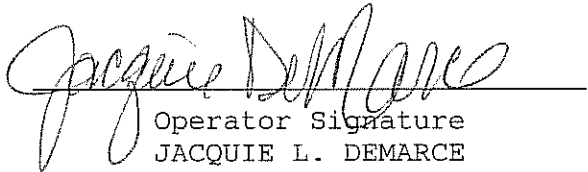
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004194  
Location = ~~TOX~~ *F70T OK*      8164.13.00 06/09  
12/18/2009      15:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:27
02 Std. Gas	0.076	15:28
03 Room Air	0.000	15:28
04 Std. Gas	0.077	15:28
05 Room Air	0.000	15:29
06 Std. Gas	0.077	15:29
07 Room Air	0.000	15:30

Lot No = 659358  
Cyl No = 56  
Exp Date = 09/03/2011  
County = 03      Oper No. = 100103

  
Operator Signature  
JACQUIE L. DEMARCE

Remarks:

Form 106-I8000

80-004194  
P. 2 of 2 KM