



ETHANOL BREATH STANDARD CYLINDER REPORT
OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Joseph Krawski</u>		
Location: <u>Devils Lake LEC</u>		
Intoxilyzer® Serial Number: <u>80-004193</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>20</u>	Expiration Date: <u>9-3-11</u>
<input type="checkbox"/> New Cylinder Installed	<input type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.082</u> %		
Test 2: <u>0.083</u> %		
Test 3: <u>0.082</u> %		
(ATTACH TEST RECORD)		

Joseph Krawski
Chemical Test Operator Signature

12-22-2010
Date

Deb Kashner
Reviewed By

16 Feb 2011
Date

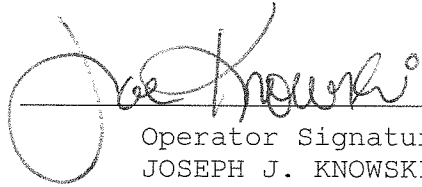
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = DEVL 8164.13.00 06/09
12/22/2010 19:33

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	19:33
02 Std. Gas	0.082	19:34
03 Room Air	0.000	19:34
04 Std. Gas	0.083	19:35
05 Room Air	0.000	19:35
06 Std. Gas	0.082	19:35
07 Room Air	0.000	19:36

Lot No = 659358
Cyl No = 20
Exp Date = 09/03/2011
County = 36 Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004193
P. 90 of 90
FM