

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Duane L. Marmor

Location: STAN

Intoxilyzer Serial No.: 80-003071

Lot Number: 659358

Cylinder Number: 43

Expiration Date: 09/03/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 078 %

Test 2: 0. 079 %

Test 3: 0. 078 %

(ATTACH TEST RECORD)

D L Marmor
Chemical Test Operator Signature

12/30/09
Date

Deb Kashur
Reviewed By

07 Jan 2010
Date

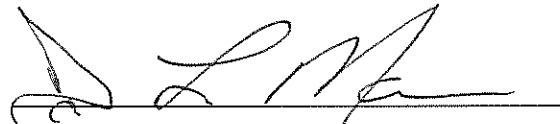
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = STAN 8164.13.00 06/09
12/30/2009 19:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	19:29
02 Std. Gas	0.078	19:29
03 Room Air	0.000	19:30
04 Std. Gas	0.079	19:30
05 Room Air	0.000	19:31
06 Std. Gas	0.078	19:31
07 Room Air	0.000	19:32

Lot No = 659358
Cyl No = 43
Exp Date = 09/03/2011
County = 31 Oper No. = 100019


Operator Signature
DUANE L. MARMON

Remarks:

Form 106-I8000

80-003071
P. 2 of 2 JPL