




ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Lori Flaten</u>		
Location: <u>Mandan PD.</u>		
Intoxilyzer® Serial Number: <u>80-004939.</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>40</u>	Expiration Date: <u>09-03-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>082</u> %		
Test 2: 0. <u>082</u> %		
Test 3: 0. <u>082</u> %		
(ATTACH TEST RECORD)		


Chemical Test Operator Signature

12-30-10
Date

Deb Kashur
Reviewed By

10 Jan 2011
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = MAND 8164.13.00 06/09
12/30/2010 10:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:15
02 Std. Gas	0.082	10:16
03 Room Air	0.000	10:16
04 Std. Gas	0.082	10:17
05 Room Air	0.000	10:17
06 Std. Gas	0.082	10:17
07 Room Air	0.000	10:18

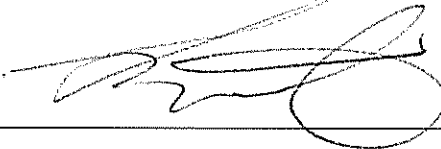
Lot No = 659358

Cyl No = 40

Exp Date = 09/03/2011

County = 30

Oper No. = 068019


Operator Signature
LORI E. FLATEN

Remarks:

Form 106-I8000

80-004939
P. 48 of 48
RM