



OFFICE OF ATTORNEY GENERAL  
 Crime Laboratory Division  
 2641 East Main Avenue  
 P.O. Box 937  
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

**ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM**

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Aaron R. Hummel

Location: GFSO

Intoxilyzer Serial No.: 80-003057

Lot Number: 659357

Cylinder Number: 26

Expiration Date: 9/3/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

*ACA Test  
 Not a change  
 of cylinder*

Test 1: 0. 082 %

Test 2: 0. 082 %

Test 3: 0. 083 %

(ATTACH TEST RECORD)

*[Signature]*  
 Chemical Test Operator Signature

12/31/09  
 Date Cylinder Changed

Deb Kashur  
 Reviewed By

07 Jan 2010  
 Date

Form 105-G  
 Toxicology Laboratory  
 Crime Laboratory Division

*80-003057  
 p. 1 of 2 ysm*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003057  
Location = GFSO      8164.13.00 06/09  
12/31/2009      14:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:57
02 Std. Gas	0.082	14:57
03 Room Air	0.000	14:58
04 Std. Gas	0.082	14:58
05 Room Air	0.000	14:58
06 Std. Gas	0.083	14:59
07 Room Air	0.000	14:59


Lot No = 659357

Cyl No = 26

Exp Date = 09/03/2011

County = 18

Oper No. = 049907

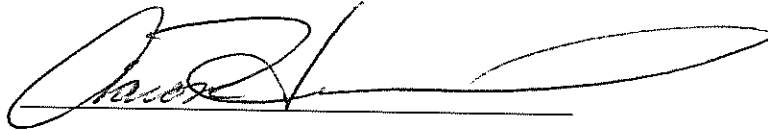

Operator Signature  
AARON HUMMEL

Remarks:

*ACA Test*

Form 106-I8000

80-003057  
P. 2 of 2 File