



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59281 (10-2016)

Serial Number <i>80-006489</i>	Instrument Location <i>GFPD</i>
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <i>was moved out of room during construction period.</i> <i>Also changed out printer.</i>	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): *installed new printer*
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>John Lampi</i>	Date <i>10-10-17</i>
--	-------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by <i>Roberta Huegel-Munro</i>	Certified Date <i>10-11-17</i>
--	-----------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006489
Location = GFPD 8164.14.00 09/16
10/10/2017 15:11

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup

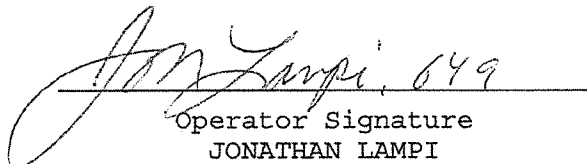
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 20016080A2
Standard Cyl #? 051
Standard Expiration? 09/05/2018
Oper No? 039947

Flow Cal. Date: 08/18/2015
Slope 663
Intercept -631787

IR Calibration Date: 08/18/2015

	3um	9um
0th Coef(*100):	-24626	-16551
1st Coef(*100):	269218	130789
2nd Coef(*100):	3390	1656
H2O adj(mg/l*10k):	742	460

***** Printer Test End *****


Operator Signature
JONATHAN LAMPI

Remarks:

104-6. Print test
new printer

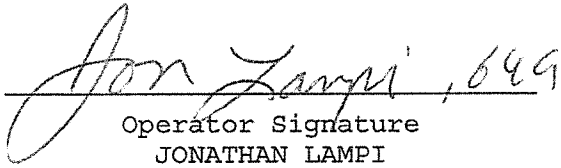
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006489
Location = GFPD 8164.14.00 09/16
10/10/2017 15:40

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:40
02 Std. Gas	0.082	15:41
03 Room Air	0.000	15:41
04 Std. Gas	0.082	15:42
05 Room Air	0.000	15:42
06 Std. Gas	0.082	15:43
07 Room Air	0.000	15:43

Lot No = 20016080A2
Cyl No = 051
Exp Date = 09/05/2018
County = 18 Oper No. = 039947


Operator Signature
JONATHAN LAMPI

Remarks:
104-G, ACA

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006489
Location = GFPD 8164.14.00 09/16
10/10/2017 15:53

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	15:54
02 Room Air	0.000	15:54

*Invalid Test
Inhibited - RFI

Lot No = 20016080A2
Cyl No = 051
Exp Date = 09/05/2018
County = 18 Oper No. = 039947


Operator Signature
JONATHAN LAMPI

Remarks:

104G Form 106-I8000
RFI Test