



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59281 (10-2016)

Serial Number 80-005945	Instrument Location New Town, ND - Justice Center
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <u>Install after update from Crime Lab. 13 Dec 17 RBN</u>	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000. N/A
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature AMT	5664	Date 12-13-2017
---	-------------	---------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by Roberta Singer-Timmer	Certified Date 12-13-2017
---	-------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = NEWT 8164.14.00 09/16
12/12/2017 16:45

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNopQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNopQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 17316080A2
Standard Cyl #? 35
Standard Expiration? 08/05/2018
Oper No? 131739

Flow Cal. Date: 06/20/2013
Slope 637
Intercept -566407

IR Calibration Date: 05/22/2015
 3um 9um

0th Coef(*100): -21213 -23093
1st Coef(*100): 279171 139292
2nd Coef(*100): 2898 1291
H2O adj(mg/l*10k): 332 319

***** Printer Test End *****

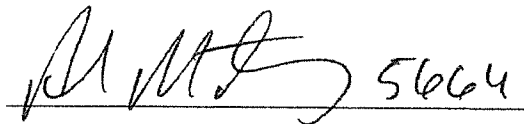

Operator Signature
ANDRES MARTINEZ

Remarks:

Install after update from Bismarck, ND.


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = NEWT 8164.14.00 09/16
12/13/2017 11:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:14
02 Std. Gas	0.080	11:14
03 Room Air	0.000	11:14
04 Std. Gas	0.080	11:15
05 Room Air	0.000	11:15
06 Std. Gas	0.080	11:16
07 Room Air	0.000	11:16

Lot No = 17316080A2
Cyl No = 35
Exp Date = 08/05/2018
County = 60 Oper No. = 131739

 5664

Operator Signature
ANDRES MARTINEZ

Remarks:

Install after update from Crime Lab.

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = NEWT 8164.14.00 09/16
12/2/2017 16:43

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:43
02 Std. Gas	0.080	16:44
03 Room Air	RFI*	16:44
04 Room Air	0.000	16:45

*Invalid Test
Inhibited - RFI

Lot No = 17316080A2
Cyl No = 35
Exp Date = 08/05/2018
County = ~~67~~ ⁶⁶ ~~Red~~ ¹²⁻¹³⁻¹⁷ Oper No. = 131739


Operator Signature
ANDRES MARTINEZ

Remarks: Install after update from Bismarck, ND