



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59281 (10-2016)

Serial Number	80-005945	Instrument Location	Justice Center New Town
Reason for Install/Repair			
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <u>updates from Crime Lab.</u>			

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000. N/A
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature	<u>[Signature]</u> 5664	Date	2-15-2018
---------------------------	-------------------------	------	-----------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by	<u>[Signature]</u>	Certified Date	2-16-2018
-----------------------	--------------------	----------------	-----------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = NEWT 8164.14.00 09/16
02/15/2018 16:18

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 17316080A2
Standard Cyl #? 35
Standard Expiration? 08/05/2018
Oper No? 131739

Flow Cal. Date: 06/20/2013
Slope 637
Intercept -566407

IR Calibration Date: 05/22/2015
 3um 9um

	3um	9um
0th Coef(*100):	-21213	-23093
1st Coef(*100):	279171	139292
2nd Coef(*100):	2898	1291
H2O adj(mg/l*10k):	332	319

***** Printer Test End *****

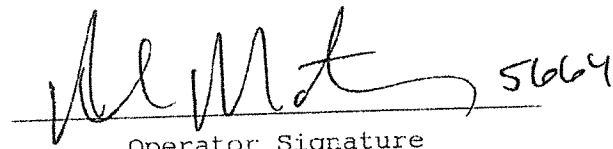

Operator Signature
ANDRES MARTINEZ

Remarks: *Install*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = NEWT 8164.14.00 09/16
02/15/2018 16:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:20
02 Std. Gas	0.081	16:20
03 Room Air	0.000	16:21
04 Std. Gas	0.081	16:21
05 Room Air	0.000	16:22
06 Std. Gas	0.081	16:22
07 Room Air	0.000	16:23

Lot No - 17316080A2
Cyl No = 35
Exp Date = 08/05/2018
County = 60 Oper No. = 131739

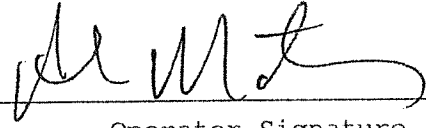
Operator Signature 5664
ANDRES MARTINEZ

Remarks: ACA Test


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = NEWT 8164.14.00 09/16
02/15/2018 16:24

Test	AC	Time
01 Room Air	0.000	16:27
02 Reference	RFI*	16:27
03 Room Air	0.000	16:28

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST TEST
Sub DOB = 12/30/1990
Sub Sex = Male Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/NA
Lot No = 17316080A2
Cyl No = 35
Expiration Date = 08/05/2018
County = 60 Oper No. = 131739

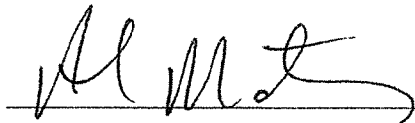

Operator Signature
ANDRES MARTINEZ

Remarks:

RFI Test