



# ETHANOL GAS STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (10-2013)

Chemical Test Operator Name (Print) <i>Robert Kennedy</i>		
Location <i>Devils Lake (LEC)</i>	Intoxilyzer® Serial Number <i>80-005954</i>	
Gas Lot Number <i>34917080A3</i>	Gas Cylinder Number <i>3</i>	Gas Expiration Date <i>2/5/2020</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).  
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).  
A. *0.080* AC  
B. *0.079* AC  
C. *0.079* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:

*rec'd at  
Crime Lab  
4/9/18 RSN*

- A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
- B. ACA Test Record.

Chemical Test Operator Signature <i>[Signature]</i>	Date <i>4/5/2018</i>
Reviewed By (Crime Laboratory Use Only) <i>[Signature]</i>	Date <i>4/9/2018</i>

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-005954  
Location = DEVL      8164.14.00 09/16  
04/05/2018      15:17

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:18
02 Std. Gas	0.080	15:18
03 Room Air	0.000	15:19
04 Std. Gas	0.079	15:19
05 Room Air	0.000	15:20
06 Std. Gas	0.079	15:20
07 Room Air	0.000	15:21


Lot No = 34917080A3

Cyl No = 3

Exp Date = 02/05/2020

County = 36

Oper No. = 069108

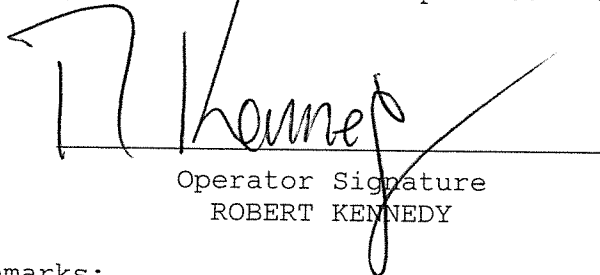

Operator Signature  
ROBERT KENNEDY

Remarks:

Form 106-I8000