

**INTOXILYZER® 8000 INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-006494

Location: BELC

BJA BELC COURT

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 912 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
  - a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.020 AC  
Sim. Ser #: DR3377 Lot #: 2016104 Exp. Date: 10.4.18
  - b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.300 AC  
Sim. Ser #: DR5191 Lot #: 17350 Exp. Date: 10.11.19

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3451 Lot #: ICS#5 Exp. Date: 5.15.19  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 63417080A3 Cyl #: 26 Exp. Date: 3.5.19

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.080</u>
Test 2	<u>0.081</u>	Test 5	<u>0.080</u>	Test 8	<u>0.081</u>
Test 3	<u>0.080</u>	Test 6	<u>0.081</u>	Test 9	<u>0.080</u>
Average	<u>0.081</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed  
Breath Analyst Signature

CEE 6.28.18  
5.9.2018  
Date

Roberta Hueque-Tumino  
Reviewed by

18  
14 May 19  
Date

15 Jun 18

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006494  
Location = BELC                 8164.14.00 09/16  
05/09/2018                       14:01

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-==|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-==|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup

Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            No  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 03417080A3  
Standard Cyl #?                26  
Standard Expiration?            03/05/2019  
Oper No?                        666666

Flow Cal. Date:                 08/18/2015  
Slope                            655  
Intercept                       -624238

IR Calibration Date:            05/10/2017  
                                  3um                        9um

-----  
0th Coef(\*100):                -28969                    -21478  
1st Coef(\*100):                256589                   140860  
2nd Coef(\*100):                2527                     1330  
H2O adj(mg/l\*10k):            655                      473

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks:

PRINT TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006494  
Location = BELC      8164.14.00 09/16  
05/09/2018      14:23

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:24
02 Std. Sol.	0.017	14:25
03 Room Air	0.000	14:25
04 Std. Sol.	0.017	14:26
05 Room Air	0.000	14:26
06 Std. Sol.	0.017	14:27
07 Room Air	0.000	14:28


08 Sim Temp = 34.0°C

Simul Ser No = DR3377

Std Sol No = 201610A

County = 63

Oper No. = 666666

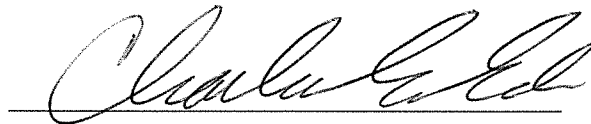

Operator Signature  
CHARLES EDER

Remarks:

Low AC  
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006494  
Location = BELC                    8164.14.00 09/16  
05/09/2018                            14:18

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:19
02 Std. Sol.	0.297	14:20
03 Room Air	0.000	14:20
04 Std. Sol.	0.297	14:21
05 Room Air	0.000	14:21
06 Std. Sol.	0.296	14:22
07 Room Air	0.000	14:23

08 Sim Temp = 34.0°C

Simul Ser No = DR5191

Std Sol No = 17350

County = 63

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.300AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006494  
Location = BELC      8164.14.00 09/16  
05/09/2018      14:05

Test	AC	Time
01 Room Air	0.000	14:06
02 *Subject Test	INT*	14:06
03 Room Air	0.000	14:07

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 03/01/1982  
Sub Sex = Male      Weight = 120  
Test = DUI      Cit = INTEREFERENT  
Dr. Lic. = ND/DIS821449  
Lot No = 03417080A3  
Cyl No = 26  
Expiration Date = 03/05/2019  
County = 63      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent Check*  
*0.10 AC + 0.05% ACETONE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006494  
Location = BELC                    8164.14.00 09/16  
05/09/2018                            14:02

Test	AC	Time
01 Diagnostic	OK	14:03
02 Room Air	0.000	14:03
03 *Subject Test	RFI*	14:04
04 Room Air	0.000	14:04

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 03/01/1982  
Sub Sex = Male                      Weight = 120  
Test = DUI                            Cit = RFI CHECK  
Dr. Lic. = ND/DIS821449  
Lot No = 03417080A3  
Cyl No = 26  
Expiration Date = 03/05/2019  
County = 63                          Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

RFI CHECK


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006494  
Location = BELC      8164.14.00 09/16  
05/09/2018      14:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:11
02 Std. Gas	0.081	14:12
03 Room Air	0.000	14:12
04 Std. Gas	0.081	14:13
05 Room Air	0.000	14:13
06 Std. Gas	0.080	14:14
07 Room Air	0.000	14:14

Lot No = 03417080A3  
Cyl No = 26  
Exp Date = 03/05/2019  
County = 63      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006494  
Location = BELC                    8164.14.00 09/16  
05/09/2018                            14:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:15
02 Std. Gas	0.081	14:15
03 Room Air	0.000	14:16
04 Std. Gas	0.080	14:16
05 Room Air	0.000	14:17
06 Std. Gas	0.081	14:17
07 Room Air	0.000	14:18

Lot No = 03417080A3  
Cyl No = 26  
Exp Date = 03/05/2019  
County = 63                            Oper No. = 666666

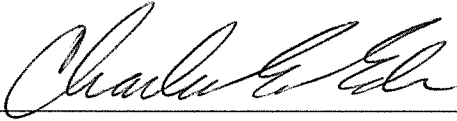  
Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-006494  
Location = BELC                              8164.14.00 09/16  
05/09/2018    14:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:29
02 Std. Gas	0.080	14:29
03 Room Air	0.000	14:30
04 Std. Gas	0.081	14:30
05 Room Air	0.000	14:31
06 Std. Gas	0.080	14:31
07 Room Air	0.000	14:32

Lot No = 03417080A3  
Cyl No = 26  
Exp Date = 03/05/2019  
County = 63                                      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC