



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59281 (10-2016)

| | |
|---|--------------------------------------|
| Serial Number <i>80-005358</i> | Instrument Location <i>UND-PD</i> |
| Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____ | |

Check When Done:

- TLM* 1. Surge Protector Installed/Properly Grounded.
- TLM* 2. Telephone Line Connected to Intoxilyzer® 8000.
- TLM* 3. Breath Tube Heated.
- TLM* 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- TLM* 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- TLM* 6. Run Tests:
 - TLM* A. Print Test (Level 1, Function P).
 - TLM* B. ACA Test (Level 1, Function C).
 - TLM* C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- TLM* 7. Repair and/or Maintenance Performed (if Any): *None*
- TLM* 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- TLM* 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- TLM* 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

| | |
|--|------------------------|
| Field Inspector Signature <i>Wayne L. Mackenzie</i> | Date <i>5-14-18</i> |
|--|------------------------|

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

| | |
|---|----------------------------------|
| Reviewed/Certified by <i>Roberta Huegu-nimmo</i> | Certified Date <i>5-24-18</i> |
|---|----------------------------------|

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = UNDP 8164.14.00 09/16
05/14/2018 15:24

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 03417080A3
Standard Cyl #? 32
Standard Expiration? 03/05/2019
Oper No? 119409

Flow Cal. Date: 04/17/2014
Slope 622
Intercept -324577

IR Calibration Date: 04/17/2015
 3um 9um

0th Coef(*100): -16867 -25778
1st Coef(*100): 266890 139601
2nd Coef(*100): 3270 1479
H2O adj(mg/l*10k): 332 443

***** Printer Test End *****


Operator Signature
TRACY MEIDINGER

Remarks:

Install 5-14-18

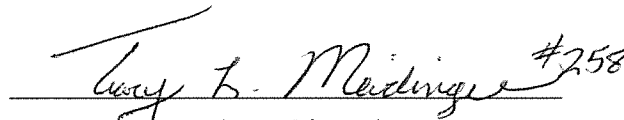
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = UNDP 8164.14.00 09/16
05/14/2018 15:25

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 15:26 |
| 02 Std. Gas | 0.079 | 15:26 |
| 03 Room Air | 0.000 | 15:27 |
| 04 Std. Gas | 0.080 | 15:27 |
| 05 Room Air | 0.000 | 15:27 |
| 06 Std. Gas | 0.080 | 15:28 |
| 07 Room Air | 0.000 | 15:28 |

Lot No = 03417080A3
Cyl No = 32
Exp Date = 03/05/2019
County = 18 Oper No. = 119409


Operator Signature
TRACY MEIDINGER

Remarks:

Install 5-14-18

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

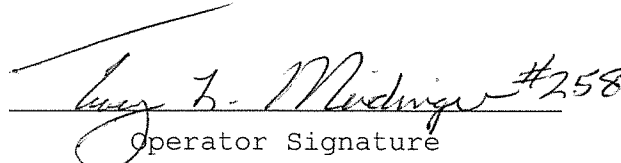
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = UNDP 8164.14.00 09/16
05/14/2018 15:30

| Test | AC | Time |
|------------------|-------|-------|
| 01 Diagnostic | OK | 15:31 |
| 02 Room Air | 0.000 | 15:32 |
| 03 *Subject Test | RFI* | 15:32 |
| 04 Room Air | 0.000 | 15:33 |

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST T
Sub DOB = 01/01/1999
Sub Sex = Male Weight = 190
Test = DUI Cit = 11111111
Dr. Lic. = ND/TES999999
Lot No = 03417080A3
Cyl No = 32
Expiration Date = 03/05/2019
County = 18 Oper No. = 119409

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.


Operator Signature
TRACY MEIDINGER

Remarks:

Install 5-14-18