



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80805945	Instrument Location McKenzie County Corrections 1201 12th ST SE Suite B
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): None
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>[Signature]</i>	Date 11/5/18
---	------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By <i>[Signature]</i>	Certified Date 11/16/18
---	-----------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = WATF 8164.14.00 09/16
11/05/2018 00:13

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

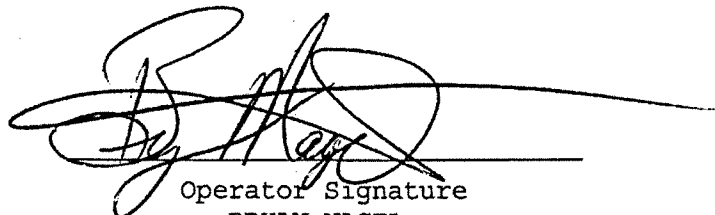
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 19817080A4
Standard Cyl #? 018
Standard Expiration? 09/05/2019
Oper No? 130626

Flow Cal. Date: 06/20/2013
Slope 637
Intercept -566407

IR Calibration Date: 05/22/2015
3um 9um

	3um	9um
0th Coef(*100):	-21213	-23093
1st Coef(*100):	279171	139292
2nd Coef(*100):	2898	1291
H2O adj(mg/l*10k):	332	319

***** Printer Test End *****



Operator Signature
BRYAN NAGEL

Remarks:

Form 106-18000

STATE OF NORTH DAKOTA }
COUNTY OF MCKENZIE }^{ss}

I certify that the foregoing is a true and correct
copy of the original document on file in this office.
Dated at Watford City, North Dakota.

on this 5th day of November 2018

McKenzie County Sheriff's Department

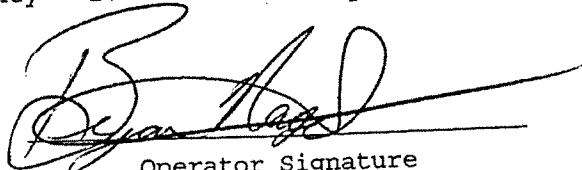
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = WATF 8164.14.00 09/16
11/05/2018 00:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	00:17
02 Std. Gas	0.078	00:18
03 Room Air	0.000	00:18
04 Std. Gas	0.077	00:18
05 Room Air	0.000	00:19
06 Std. Gas	0.078	00:19
07 Room Air	0.000	00:20

Lot No = 19817080A4
Cyl No = 018
Exp Date = 09/05/2019
County = 27 Oper No. = 130626



Operator Signature
BRYAN NAGEL

Remarks:

Form 106-I8000

STATE OF NORTH DAKOTA }
COUNTY OF MCKENZIE }^{ss}

I certify that the foregoing is a true and correct
copy of the original document on file in this office.
Dated at Watford City, North Dakota.

on this 5th day of November 2018

Mckenzie County Sheriff's Department

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

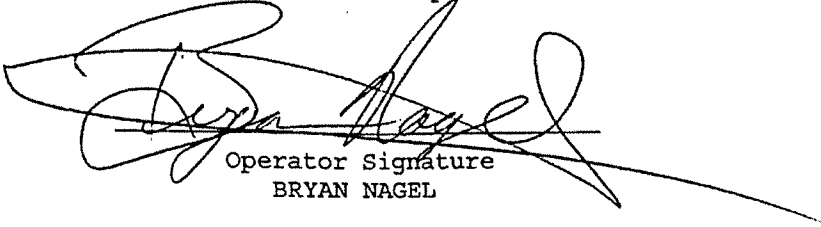
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005945
Location = WATF 8164.14.00 09/16
11/05/2018 00:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	00:27
02 Room Air	RFI*	00:28

*Invalid Test
Inhibited - RFI

Lot No = 19817080A4 Oper No. = 130626
Cyl No = 018
Exp Date = 09/05/2019
County = 27


Operator Signature
BRYAN NAGEL

Remarks:

Form 106-I8000

STATE OF NORTH DAKOTA }
COUNTY OF MCKENZIE }

I certify that the foregoing is a true and correct
copy of the original document on file in this office.
Dated at Watford City, North Dakota.

on this 5th day of November 2018


McKenzie County Sheriff's Department