



ETHANOL GAS STANDARD CYLINDER REPORT

NORTH DAKOTA OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM

SFN 59282 (08/2018)

Chemical Test Operator Name (Print) <i>Tracy L. Meidinger</i>		
Location <i>UNDP</i>	Intoxilyzer® Serial Number <i>80-005358</i>	
Gas Lot Number <i>13518080A6</i>	Gas Cylinder Number <i>17</i>	Gas Expiration Date <i>08-05-2020</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. *0.081* AC
 - B. *0.080* AC
 - C. *0.082* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Tracy L. Meidinger</i>	Date <i>12-10-2018</i>
Reviewed By (Crime Laboratory Use Only) <i>Roberta Huger-Nimmo</i>	Date <i>12-20-2018</i>

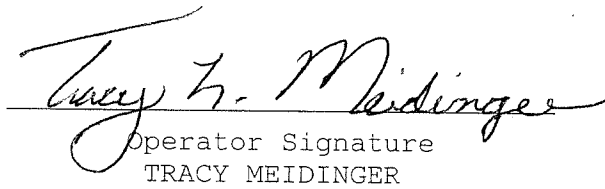
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = UNDP 8164.14.00 09/16
12/10/2018 13:40

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:41
02 Std. Gas	0.081	13:41
03 Room Air	0.000	13:41
04 Std. Gas	0.080	13:42
05 Room Air	0.000	13:42
06 Std. Gas	0.082	13:43
07 Room Air	0.000	13:43

Lot No = 13518080A6
Cyl No = 17
Exp Date = 08/05/2020
County = 18 Oper No. = 119409


Operator Signature
TRACY MEIDINGER

Remarks:

Form 106-I8000